

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024827.D
 Acq On : 11 Oct 2022 00:34
 Operator : SY/VA
 Sample : N5064-03
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BJ3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 11 02:01:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	491882	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	374511	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	114370	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	100861	19.598	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.400%		
7) Chloroethane-d5	2.879	69	60206	20.132	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.520%		
11) 1,1-Dichloroethene-d2	4.013	63	155902m	13.088	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.360%		
21) 2-Butanone-d5	7.080	46	75537	40.825	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.660%		
24) Chloroform-d	7.647	84	295772	22.492	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.960%		
26) 1,2-Dichloroethane-d4	8.305	65	164193m	24.070	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.280%		
32) Benzene-d6	8.275	84	538093	22.479	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.920%		
36) 1,2-Dichloropropane-d6	9.274	67	188822	25.817	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.280%		
41) Toluene-d8	10.323	98	410873	19.205	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.800%		
43) trans-1,3-Dichloroprop...	10.579	79	47006	14.432	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	57.720%		
47) 2-Hexanone-d5	10.920	63	53663	42.884	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.760%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	136304	26.156	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	83478	20.742	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.960%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	4102	3.039	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024827.D
Acq On : 11 Oct 2022 00:34
Operator : SY/VA
Sample : N5064-03
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0BJ3

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 10/11/2022
Supervised By : Mahesh Dadoda 10/11/2022


Quant Time: Oct 11 02:01:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

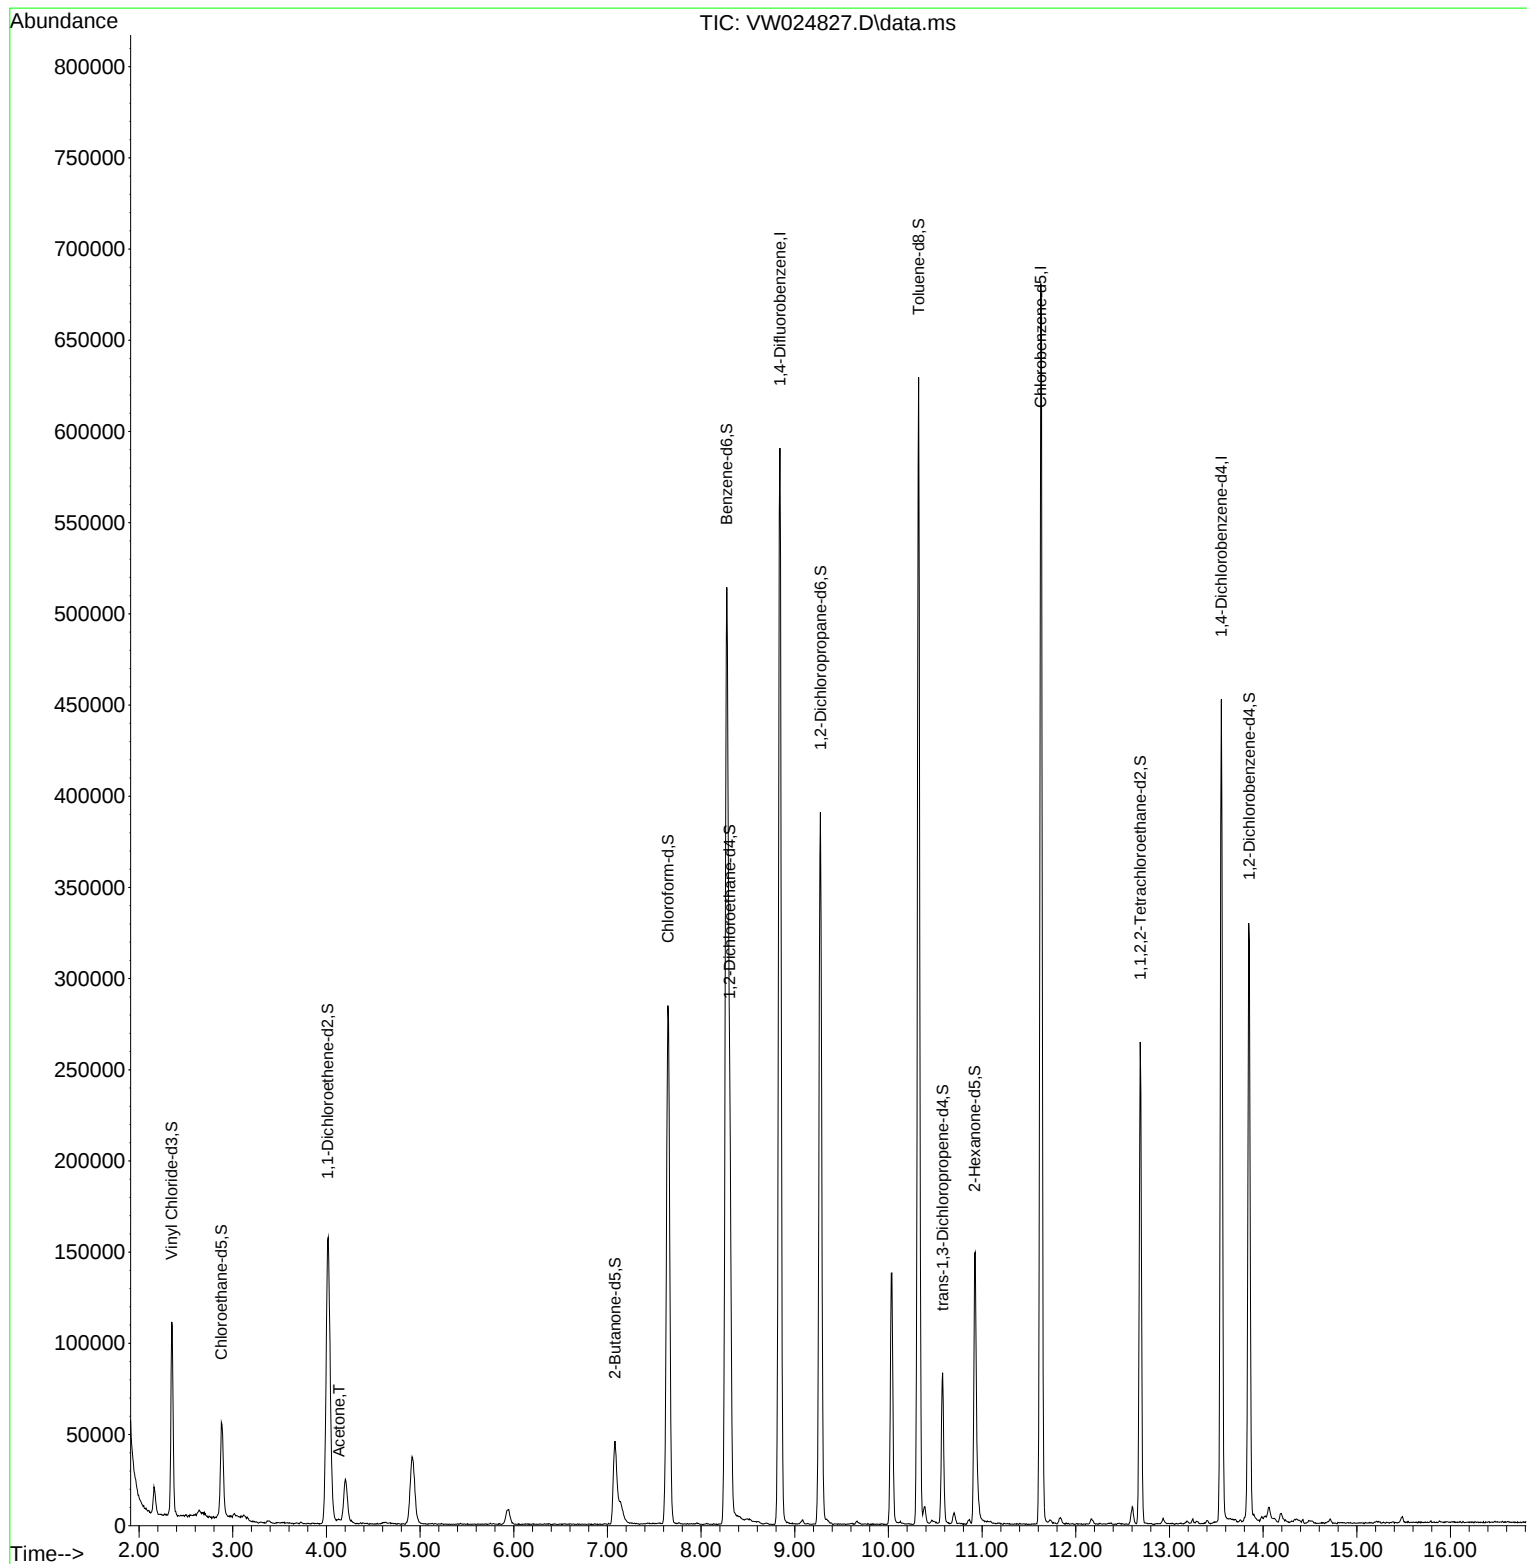

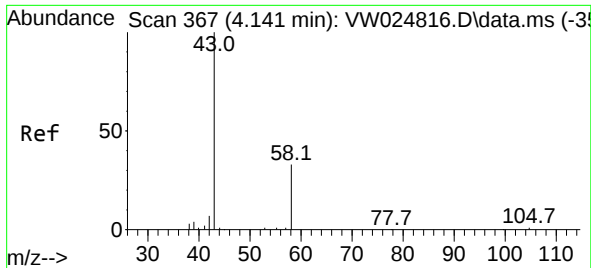

#13
 Acetone
 Concen: 3.039 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW024827.D
 Acq: 11 Oct 2022 00:34

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BJ3

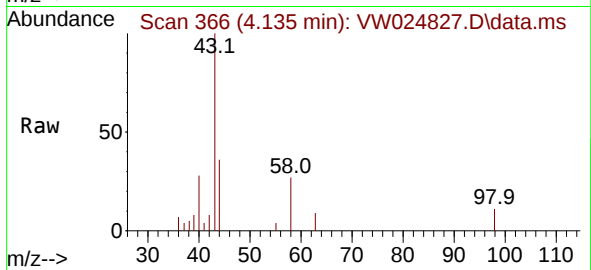

Tgt Ion: 43 Resp: 410
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 67.6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

