

Data File : VW013536.D
Acq On : 11 Oct 2019 14:28
Operator : SY/VA
Sample : K5265-21RE
Misc : 4.75G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBAT3

Quant Time: Oct 11 22:34:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 22:30:37 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	448268	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	351106	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	127973	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	94512	18.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.68%
7) Chloroethane-d5	2.89	69	83313	21.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.60%
10) 1,1-Dichloroethene-d2	4.01	63	152714	14.34	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.36%
20) 2-Butanone-d5	7.08	46	65190	42.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.36%
24) Chloroform-d	7.65	84	223878	22.99	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.96%
26) 1,2-Dichloroethane-d4	8.41	65	73	0.01	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.27	84	463091	24.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.48%
33) 1,2-Dichloropropane-d6	9.27	67	145582	26.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.36%
37) Toluene-d8	10.32	98	412646	23.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.44%
38) trans-1,3-Dichloropropene-	10.58	79	51842	20.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.44%
39) 2-Hexanone-d5	10.93	63	48742	43.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	103742	23.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.76%
61) 1,2-Dichlorobenzene-d4	13.85	152	108494	23.59	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.36%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	13.56	75	13575	3.967	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW013536.D
Acq On : 11 Oct 2019 14:28
Operator : SY/VA
Sample : K5265-21RE
Misc : 4.75G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBAT3

Quant Time: Oct 11 22:34:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 22:30:37 2019
Response via : Initial Calibration

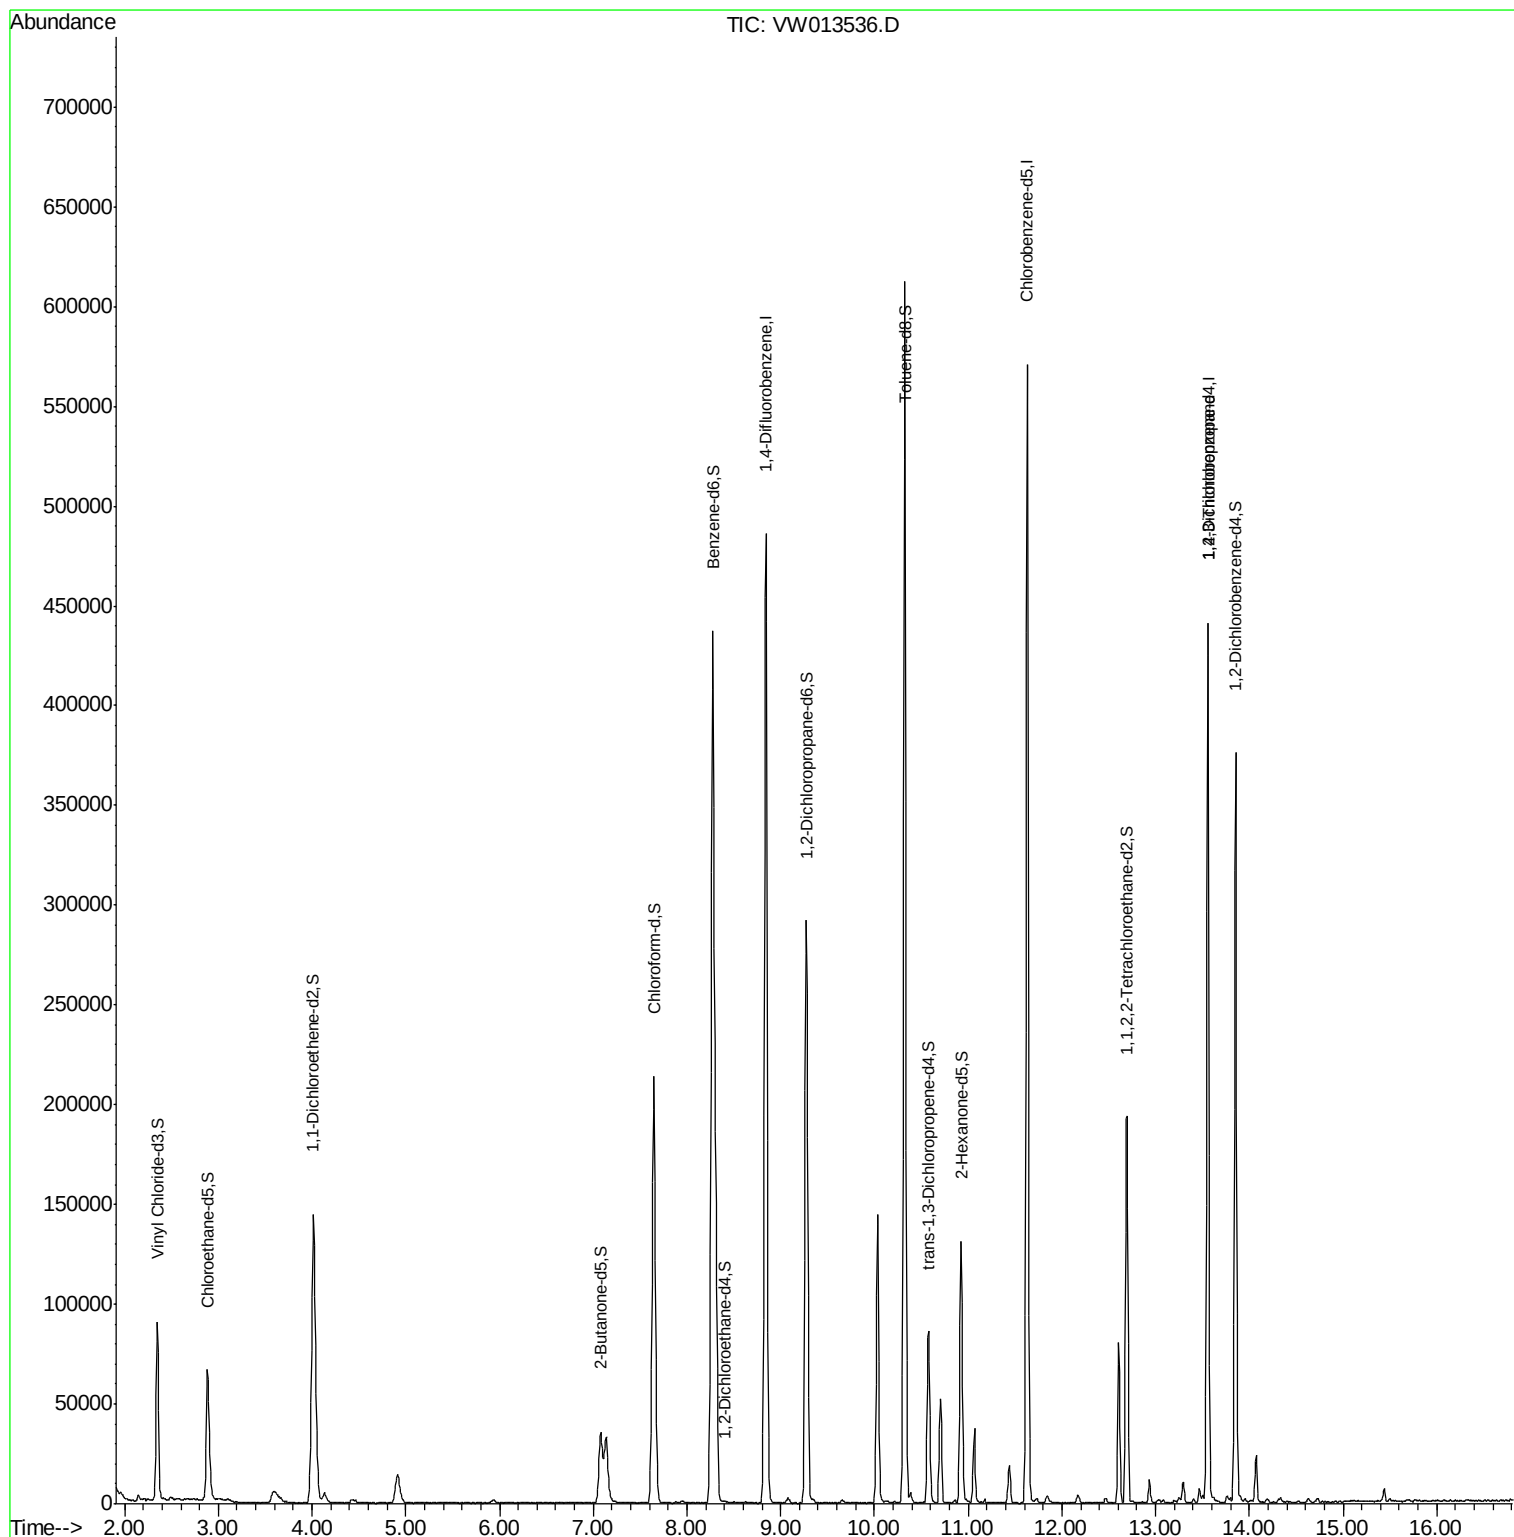

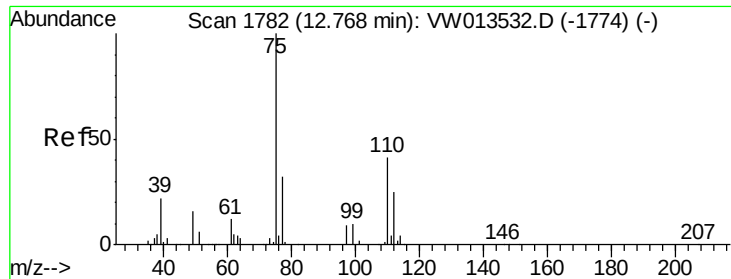

#59

1,2,3-Trichloropropane

Concen: 3.967 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW013536.D

Acq: 11 Oct 2019 14:28

Instrument :

MSVOA_W

ClientSampleId :

DBAT3

Tgt Ion: 75 Resp: 13575

Ion Ratio Lower Upper

75 100

77 34.7 25.5 38.3

