

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
 Data File : VW020434.D
 Acq On : 11 Oct 2021 10:59
 Operator : SY/VA
 Sample : M4126-16
 Misc : 3.23g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

MMDadoda

10/13/2021 10:11:47 AM

Quant Time: Oct 12 01:23:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 12 01:21:43 2021
 Response via : Initial Calibration

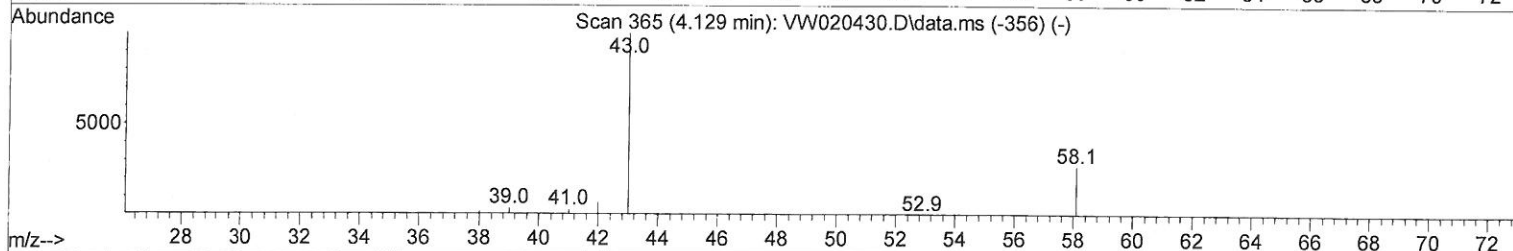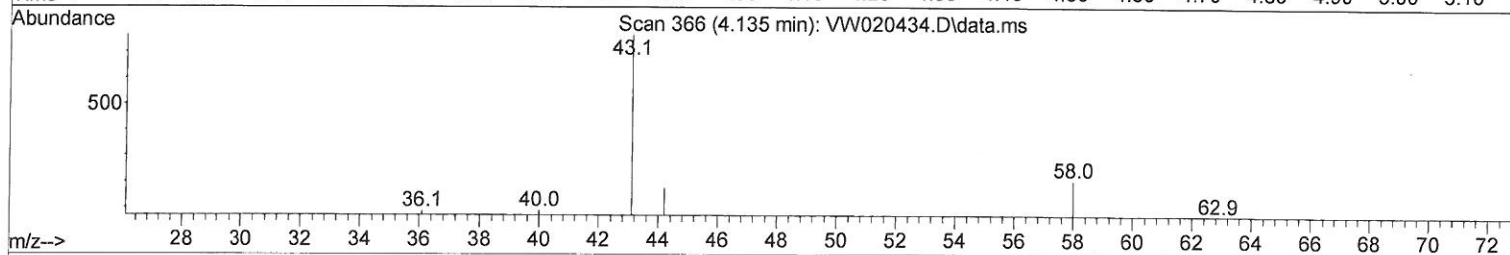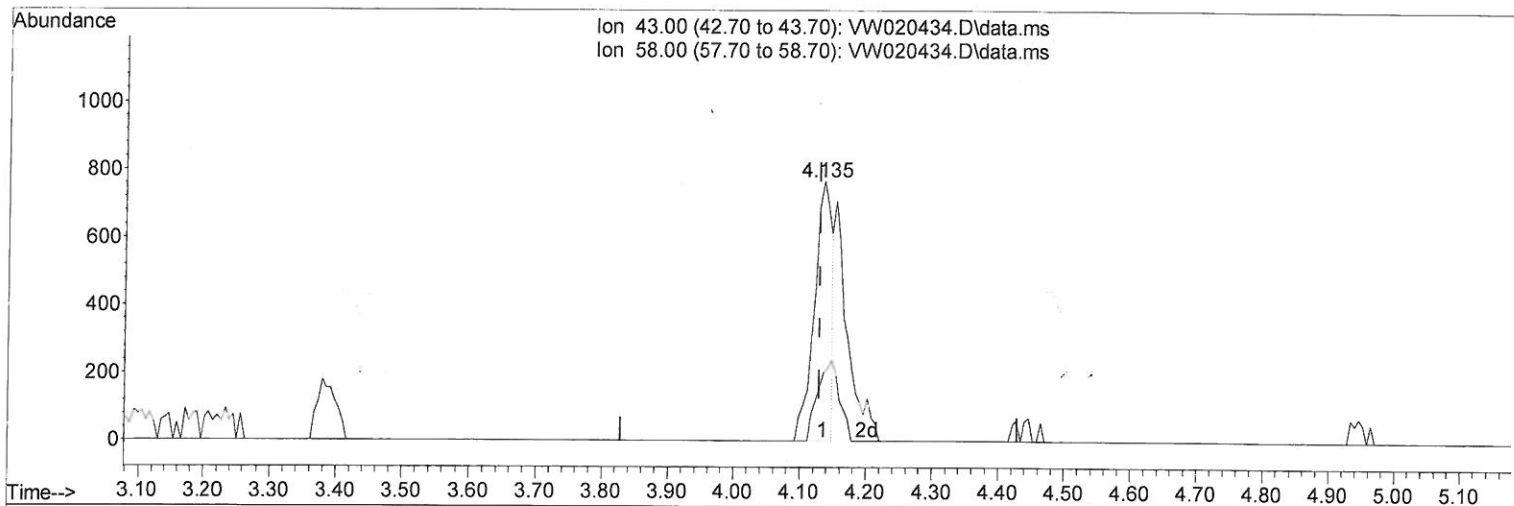

TIC: VW020434.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 2.60 ug/L

response 1411

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	38.77
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
 Data File : VW020434.D
 Acq On : 11 Oct 2021 10:59
 Operator : SY/VA
 Sample : M4126-16
 Misc : 3.23g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

MMDadoda

10/13/2021 10:11:47 AM

Quant Time: Oct 12 01:23:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 12 01:21:43 2021
 Response via : Initial Calibration

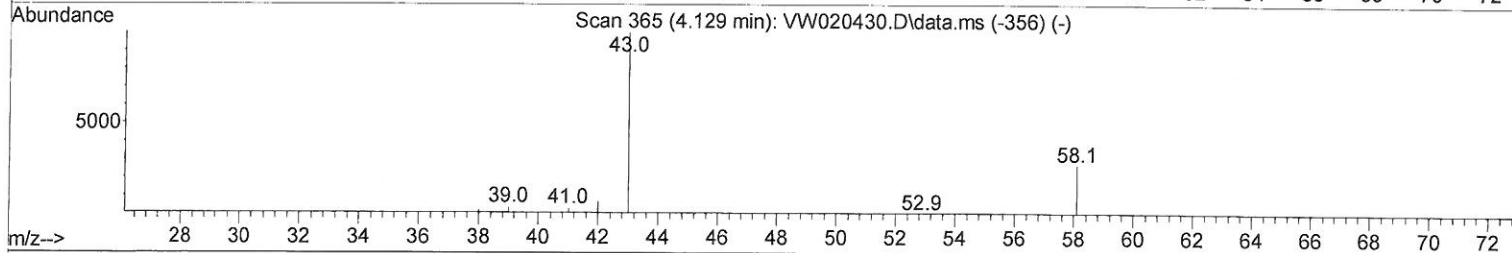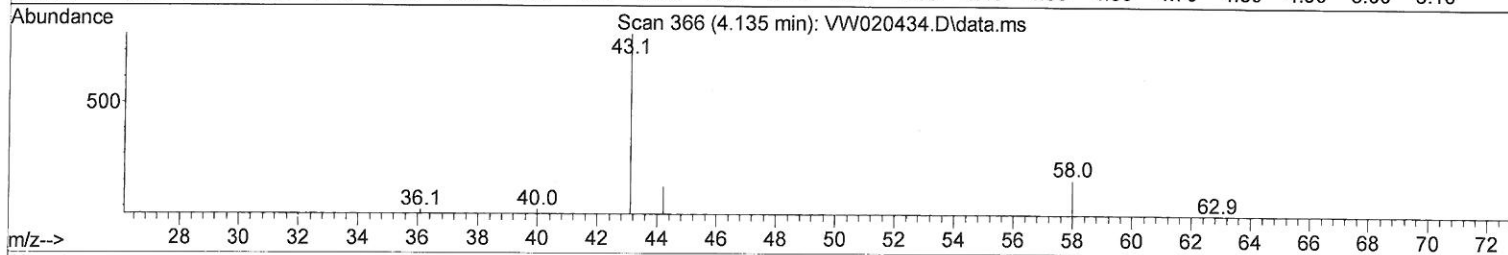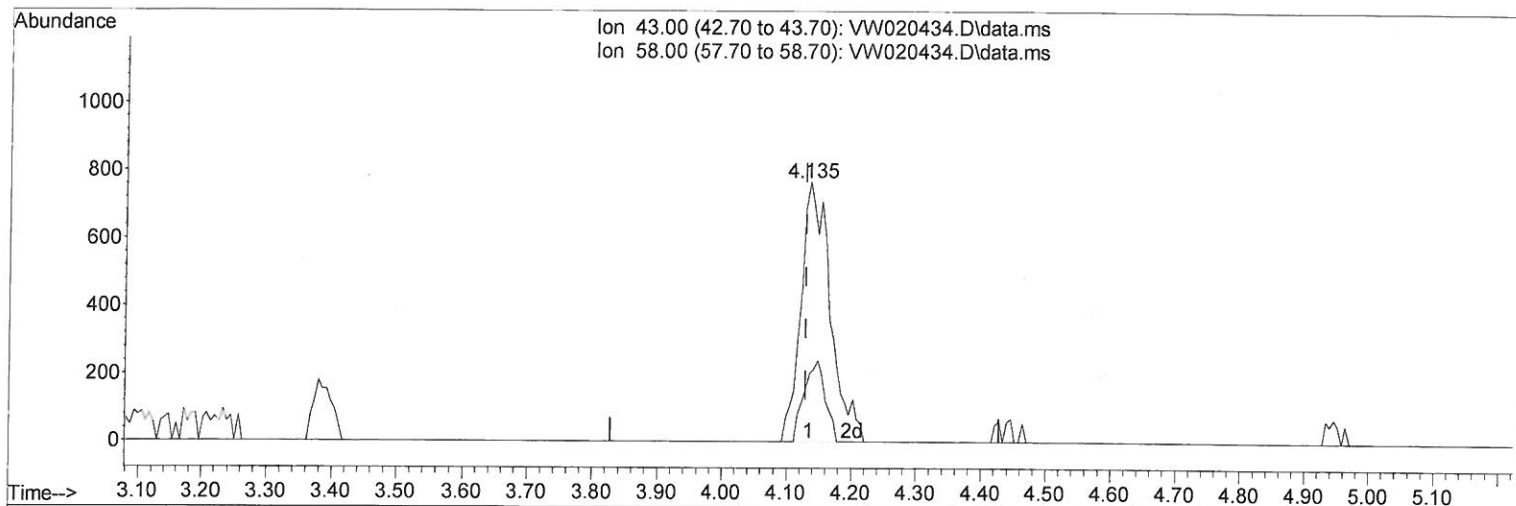

TIC: VW020434.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 4.47 ug/L m

response 2423

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.20	22.58
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
 Data File : VW020434.D
 Acq On : 11 Oct 2021 10:59
 Operator : SY/VA
 Sample : M4126-16
 Misc : 3.23g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

MMDadoda

10/13/2021 10:11:47 AM

Quant Time: Oct 12 01:23:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 12 01:21:43 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	133410	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	38651	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	4650	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	74157	38.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 152.800%#		
7) Chloroethane-d5		2.885	69	41129	40.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 160.440%#		
11) 1,1-Dichloroethene-d2		4.013	63	106841	26.860	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 107.440%		
21) 2-Butanone-d5		7.080	46	38990	65.996	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 132.000%		
24) Chloroform-d		7.647	84	152923	35.960	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 143.840%		
26) 1,2-Dichloroethane-d4		8.305	65	76971	31.691	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 126.760%		
32) Benzene-d6		8.275	84	227367	89.430	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 357.720%#		
36) 1,2-Dichloropropane-d6		9.274	67	93648	113.019	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 452.080%#		
41) Toluene-d8		10.323	98	107352	47.060	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 188.240%#		
43) trans-1,3-Dichloroprop...		10.579	79	11381	33.800	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 135.200%#		
47) 2-Hexanone-d5		10.927	63	16665	130.740	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 261.480%#		
56) 1,1,2,2-Tetrachloroeth...		12.695	84	27839	44.448	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 177.800%#		
66) 1,2-Dichlorobenzene-d4		13.853	152	4770	26.223	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 104.880%		
Target Compounds							Qvalue
13) Acetone		4.135	43	2423m	4.467	ug/L	96
16) Methylene chloride		4.909	84	11656	4.494	ug/L	96
34) Trichloroethene		9.092	95	6082	8.968	ug/L	96
46) Tetrachloroethene		10.866	164	306	0.628	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
Data File : VW020434.D
Acq On : 11 Oct 2021 10:59
Operator : SY/VA
Sample : M4126-16
Misc : 3.23g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

MMDadoda

10/13/2021 10:11:47 AM

Quant Time: Oct 12 01:23:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 12 01:21:43 2021
Response via : Initial Calibration

