

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
 Data File : VW020444.D
 Acq On : 11 Oct 2021 15:52
 Operator : SY/VA
 Sample : VIBLK472
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK472

Quant Time: Oct 12 01:25:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 12 01:21:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	294397	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	277337	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	139272	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	79680	18.600	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.400%
7) Chloroethane-d5	2.885	69	42112	18.610	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.440%
11) 1,1-Dichloroethene-d2	4.013	63	130660	14.885	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.560%
21) 2-Butanone-d5	7.086	46	56390	43.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.500%
24) Chloroform-d	7.647	84	185145	19.729	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.920%
26) 1,2-Dichloroethane-d4	8.305	65	109027	20.342	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.360%
32) Benzene-d6	8.275	84	369549	20.257	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.040%
36) 1,2-Dichloropropane-d6	9.274	67	120610	20.286	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.160%
41) Toluene-d8	10.323	98	341242	20.848	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.400%
43) trans-1,3-Dichloroprop...	10.579	79	50508	20.905	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.600%
47) 2-Hexanone-d5	10.927	63	40123	43.868	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.740%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	90946	20.237	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	115453	21.192	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.760%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	25520	4.459	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
Data File : VW020444.D
Acq On : 11 Oct 2021 15:52
Operator : SY/VA
Sample : VIBLK472
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK472

Quant Time: Oct 12 01:25:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 12 01:21:43 2021
Response via : Initial Calibration

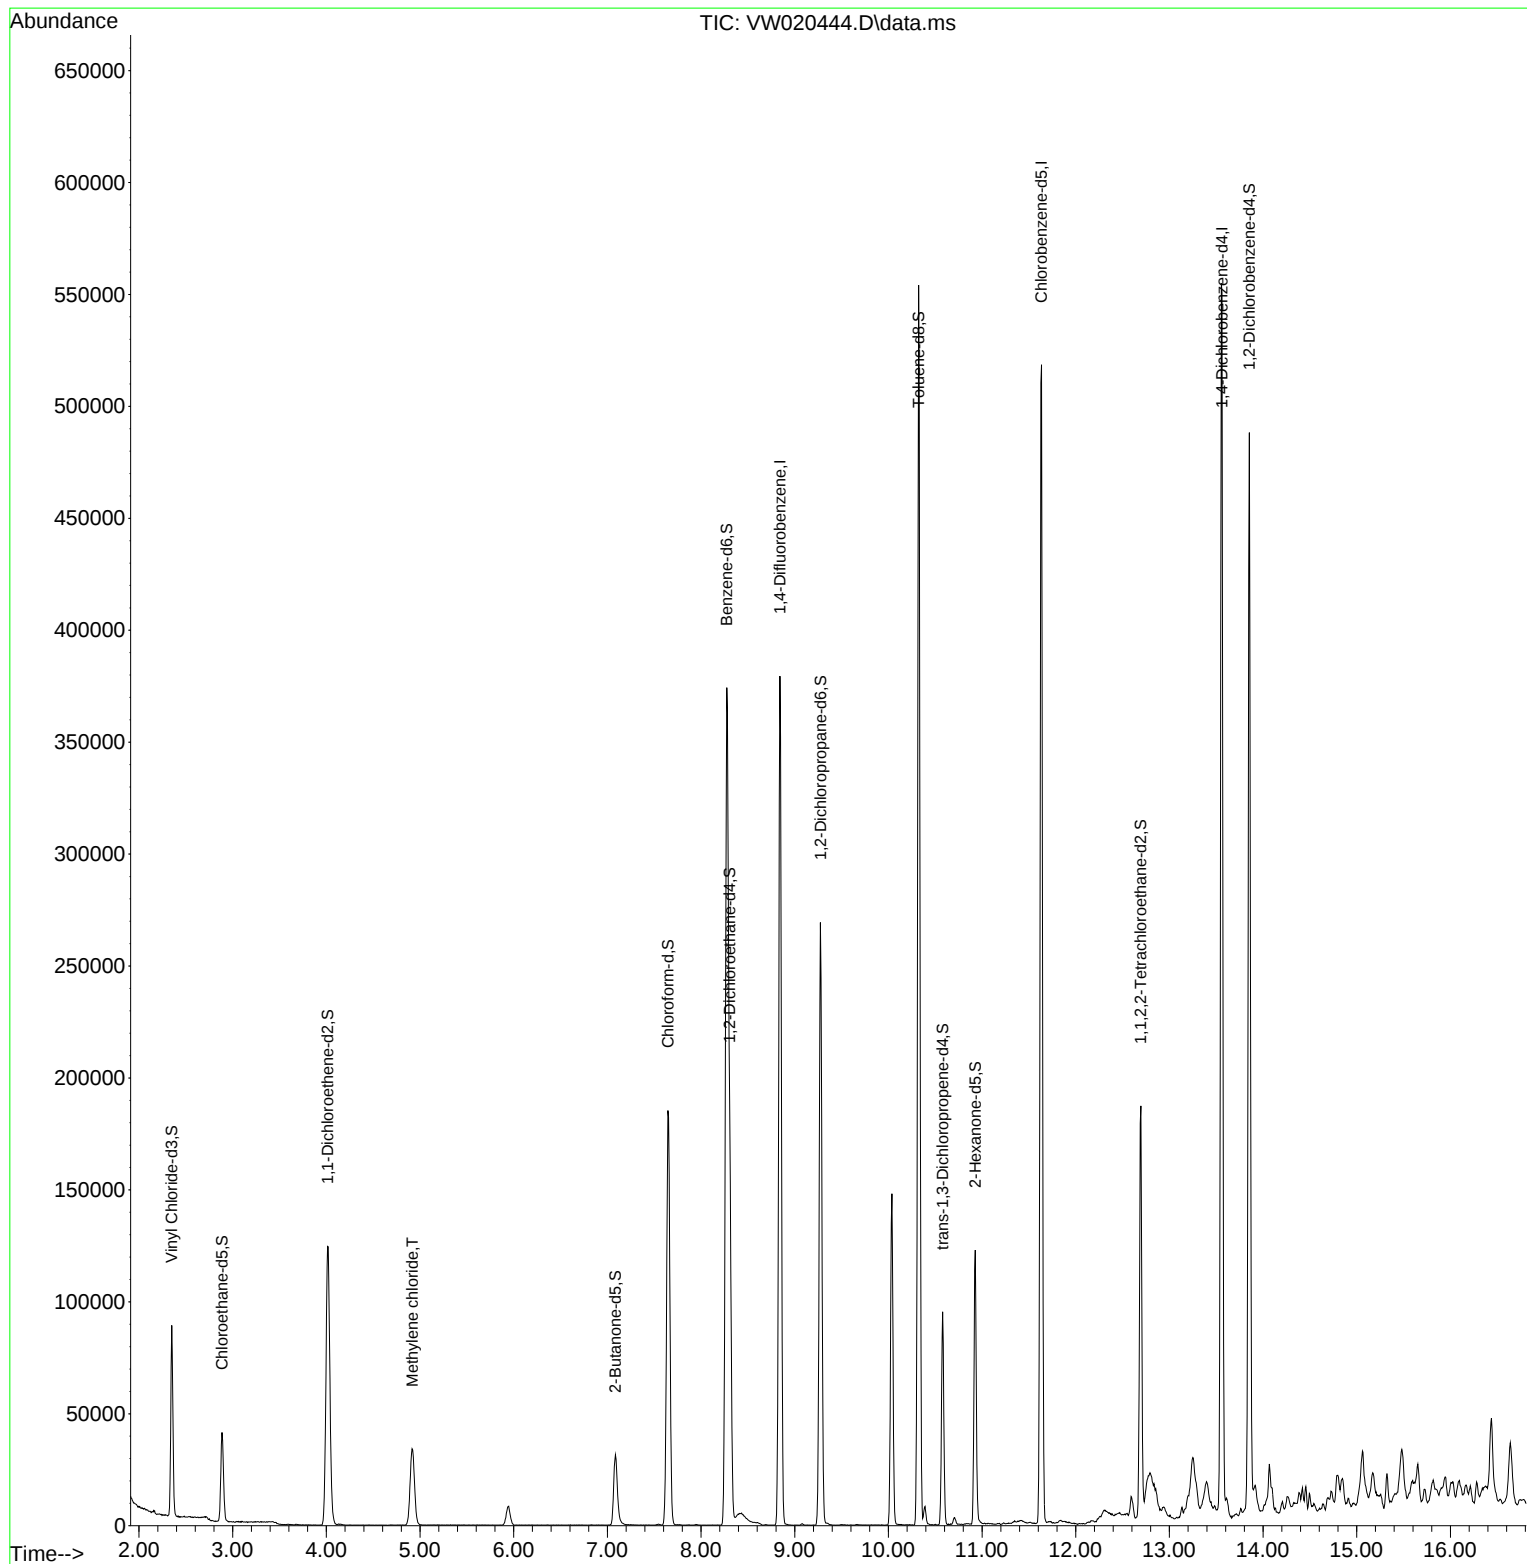

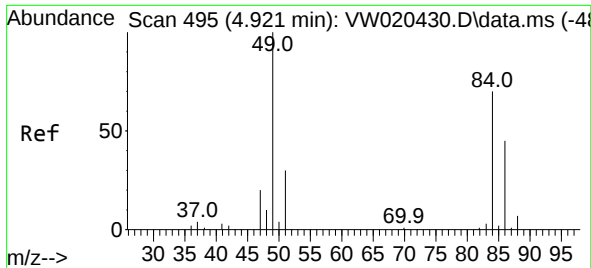

#16
Methylene chloride
Concen: 4.459 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW020444.D
Acq: 11 Oct 2021 15:52

Instrument :
MSVOA_W
ClientSampleId :
VIBLK472

Tgt Ion: 84 Resp: 25520
Ion Ratio Lower Upper
84 100
86 63.1 44.7 83.1
49 147.7 101.7 188.9

