
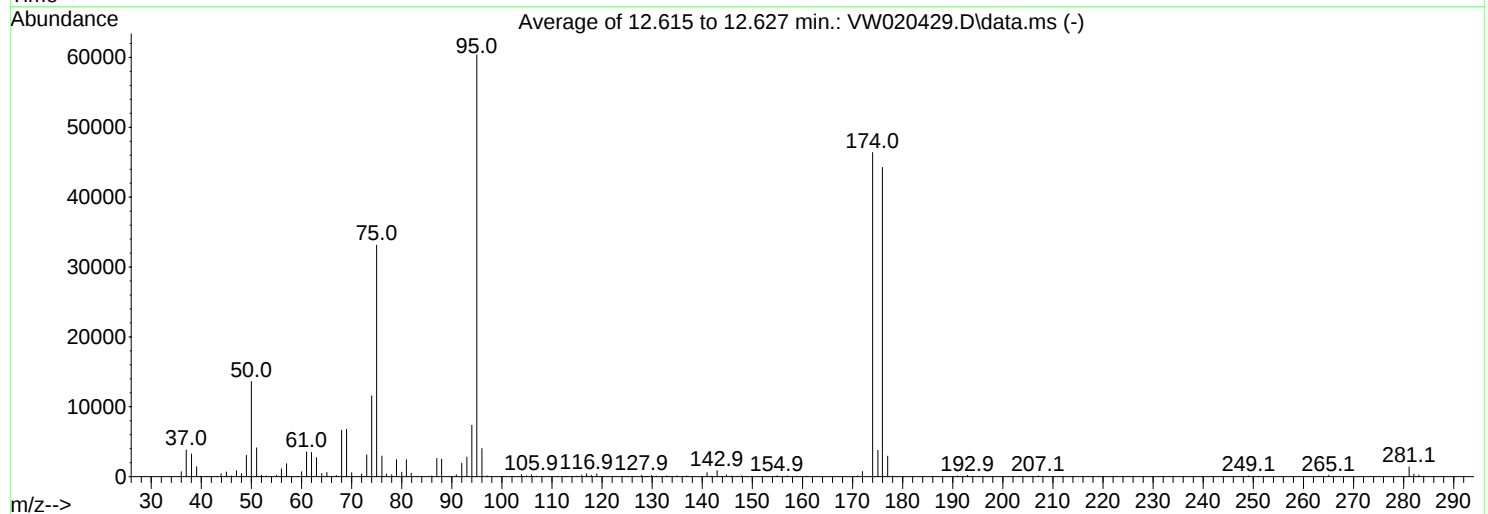


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101121\
 Data File : VW020429.D
 Acq On : 11 Oct 2021 07:39
 Operator : SY/VA
 Sample : BFB449
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB449

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Thu Oct 14 00:58:33 2021

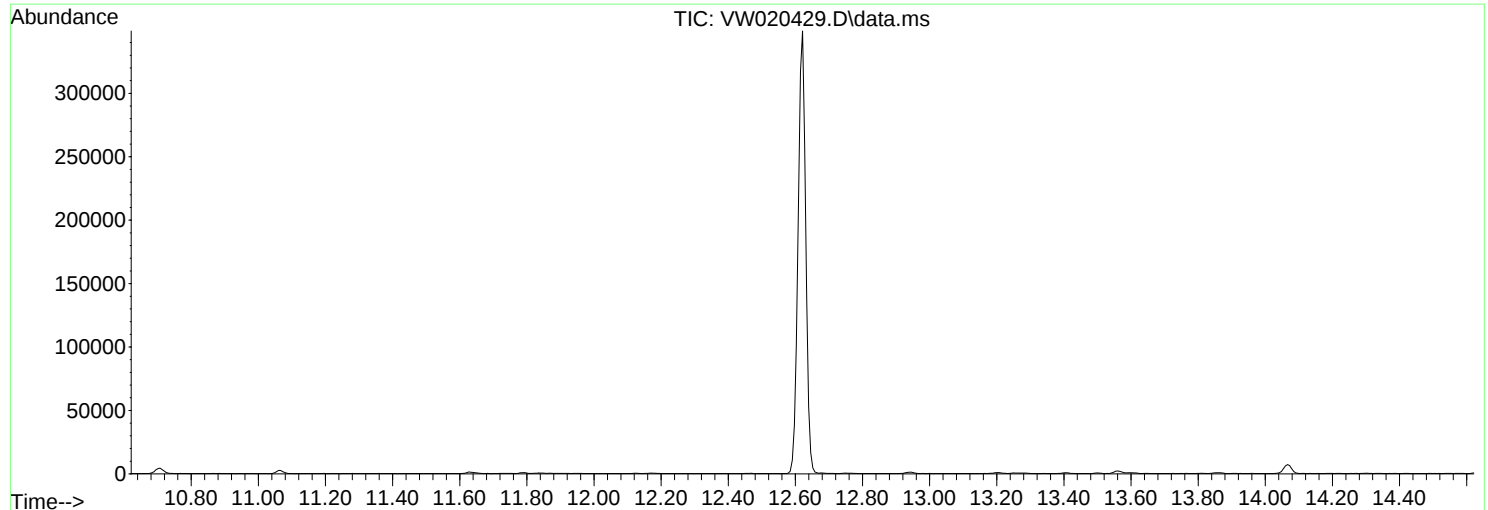

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	13610	PASS
75	95	30	80	54.9	33125	PASS
95	95	100	100	100.0	60368	PASS
96	95	5	9	6.7	4024	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.9	46395	PASS
175	174	5	9	8.1	3768	PASS
176	174	95	105	95.4	44253	PASS
177	176	5	10	6.6	2924	PASS

m/z	Abundance
39.90	116.0
43.90	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	778.0
37.00	4276.0
38.00	3689.0
39.00	1729.0
40.00	168.0
41.00	68.0
43.00	70.0
44.00	617.0
45.00	748.0
46.00	124.0
47.00	838.0
48.00	504.0
49.00	3442.0
50.00	14946.0
51.10	4386.0
52.00	234.0
52.90	102.0
55.00	194.0
56.00	1172.0
57.00	2054.0
58.10	64.0
59.10	84.0
60.00	785.0
61.00	3742.0
62.00	3732.0
63.00	2968.0
64.00	554.0
65.00	679.0
66.10	84.0
67.00	164.0
68.00	7051.0
69.00	7252.0
70.00	693.0
72.00	420.0
73.00	3294.0
74.00	12272.0
75.00	35784.0
76.10	3330.0
77.00	448.0
78.00	311.0
78.90	2693.0
80.00	713.0
80.90	2593.0
81.90	547.0
86.00	170.0
87.00	2667.0
87.90	2607.0
90.90	264.0
92.00	1987.0
93.00	3089.0
94.00	8056.0
95.00	62208.0
96.00	4442.0
97.00	91.0
103.90	280.0
104.90	114.0
105.90	293.0
106.90	83.0
112.70	61.0
114.90	69.0
115.90	197.0
116.90	454.0
117.80	178.0
118.90	443.0
125.00	83.0
127.90	235.0
128.90	100.0
129.80	193.0
131.00	98.0
132.80	252.0
135.00	138.0
136.90	117.0
140.90	575.0
141.80	73.0
143.00	860.0
144.90	288.0
145.80	122.0
146.90	79.0
147.90	151.0
149.00	63.0
154.90	112.0
156.90	92.0
158.90	72.0
160.80	124.0
171.00	190.0
172.00	814.0
174.00	43264.0
175.00	3656.0
176.00	39808.0
177.00	2903.0
178.10	114.0
178.90	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

191.00	160.0
193.00	307.0
207.00	189.0
249.10	168.0
251.00	85.0
265.00	252.0
281.10	2084.0
282.10	560.0
283.10	350.0
284.00	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	781.0
37.00	4290.0
38.00	3648.0
39.10	1477.0
40.10	186.0
44.00	561.0
45.00	744.0
46.10	117.0
47.00	951.0
48.00	549.0
49.00	3220.0
50.00	15360.0
51.00	4586.0
52.00	190.0
53.00	72.0
55.00	234.0
56.00	1290.0
57.00	2074.0
58.10	72.0
60.10	838.0
61.00	3938.0
62.00	3983.0
63.00	3195.0
64.10	428.0
65.10	711.0
66.10	92.0
66.90	216.0
68.00	7763.0
69.00	7827.0
70.00	673.0
72.00	387.0
73.00	3542.0
74.00	13075.0
75.00	36896.0
76.00	3118.0
77.00	386.0
77.90	299.0
78.90	2753.0
80.00	743.0
81.00	2800.0
81.90	601.0
83.00	81.0
85.80	120.0
87.00	2864.0
88.00	2799.0
90.90	362.0
92.00	2187.0
93.00	3042.0
94.00	8133.0
95.00	68168.0
96.00	4240.0
97.10	130.0
103.90	360.0
104.90	152.0
105.90	287.0
106.90	56.0
111.10	74.0
112.70	70.0
114.90	110.0
116.00	306.0
116.90	478.0
117.90	266.0
119.00	440.0
127.90	232.0
129.00	117.0
129.90	209.0
131.00	86.0
133.00	132.0
134.90	146.0
136.90	105.0
140.00	58.0
140.90	635.0
141.80	90.0
143.00	946.0
144.80	284.0
145.90	103.0
147.00	68.0
147.90	152.0
148.80	76.0
149.90	56.0
154.90	201.0
156.90	111.0
158.80	68.0
160.90	77.0
171.00	140.0
172.00	737.0
174.00	52784.0
175.10	4290.0
176.00	51840.0
177.00	3283.0
178.00	108.0
190.90	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

192.90	141.0
207.10	77.0
249.10	79.0
251.00	55.0
265.10	215.0
281.10	1340.0
282.00	368.0
283.00	235.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	551.0
37.00	2932.0
38.10	2452.0
39.00	1052.0
40.00	176.0
43.10	55.0
44.00	447.0
45.00	488.0
46.00	98.0
47.00	738.0
48.00	271.0
49.00	2493.0
50.00	10525.0
51.00	3385.0
52.00	185.0
53.00	76.0
55.00	174.0
56.00	901.0
57.00	1448.0
59.90	495.0
61.00	2956.0
62.00	2671.0
63.00	2045.0
64.10	385.0
65.00	380.0
65.90	62.0
66.90	158.0
68.00	5092.0
69.00	5226.0
70.00	355.0
72.00	350.0
73.00	2541.0
74.00	9341.0
75.00	26696.0
76.00	2407.0
76.90	332.0
78.10	207.0
79.00	1868.0
80.00	486.0
80.90	1916.0
81.90	365.0
83.00	61.0
85.80	67.0
87.00	2283.0
88.00	2104.0
90.90	198.0
92.00	1626.0
93.00	2284.0
94.00	5852.0
95.00	50728.0
96.00	3389.0
97.00	90.0
103.90	277.0
104.90	88.0
105.90	256.0
106.90	53.0
112.90	52.0
114.90	64.0
115.90	205.0
116.90	334.0
117.90	197.0
118.90	316.0
128.00	136.0
128.70	71.0
129.90	175.0
130.80	120.0
133.00	75.0
134.90	89.0
136.90	114.0
141.00	500.0
141.90	66.0
142.90	787.0
144.90	188.0
146.00	85.0
147.00	60.0
147.80	137.0
154.90	120.0
157.00	114.0
158.80	79.0
171.90	621.0
174.00	43136.0
175.10	3357.0
175.90	41112.0
177.00	2586.0
177.90	56.0
192.90	84.0
207.10	52.0
249.10	69.0
265.00	73.0
281.00	743.0
282.10	180.0
283.00	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449