

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
 Data File : VW024841.D
 Acq On : 11 Oct 2022 11:15
 Operator : SY/VA
 Sample : N4991-17
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Oct 12 01:19:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	529386	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	480122	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	216410	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	141612	25.567	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.280%
7) Chloroethane-d5	2.885	69	78260	24.315	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.240%
11) 1,1-Dichloroethene-d2	4.019	63	222881	17.386	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.560%
21) 2-Butanone-d5	7.080	46	87683	44.032	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.060%
24) Chloroform-d	7.647	84	329228	23.263	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.040%
26) 1,2-Dichloroethane-d4	8.305	65	173810	23.675	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.680%
32) Benzene-d6	8.275	84	711548	23.187	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.760%
36) 1,2-Dichloropropane-d6	9.275	67	213237	22.742	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.960%
41) Toluene-d8	10.323	98	645733	23.543	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.160%
43) trans-1,3-Dichloroprop...	10.579	79	78485	18.797	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.200%
47) 2-Hexanone-d5	10.921	63	69881	43.560	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.120%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	157234	23.535	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	188046	24.693	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	6225	0.475	ug/L	# 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024841.D
Acq On : 11 Oct 2022 11:15
Operator : SY/VA
Sample : N4991-17
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Oct 12 01:19:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

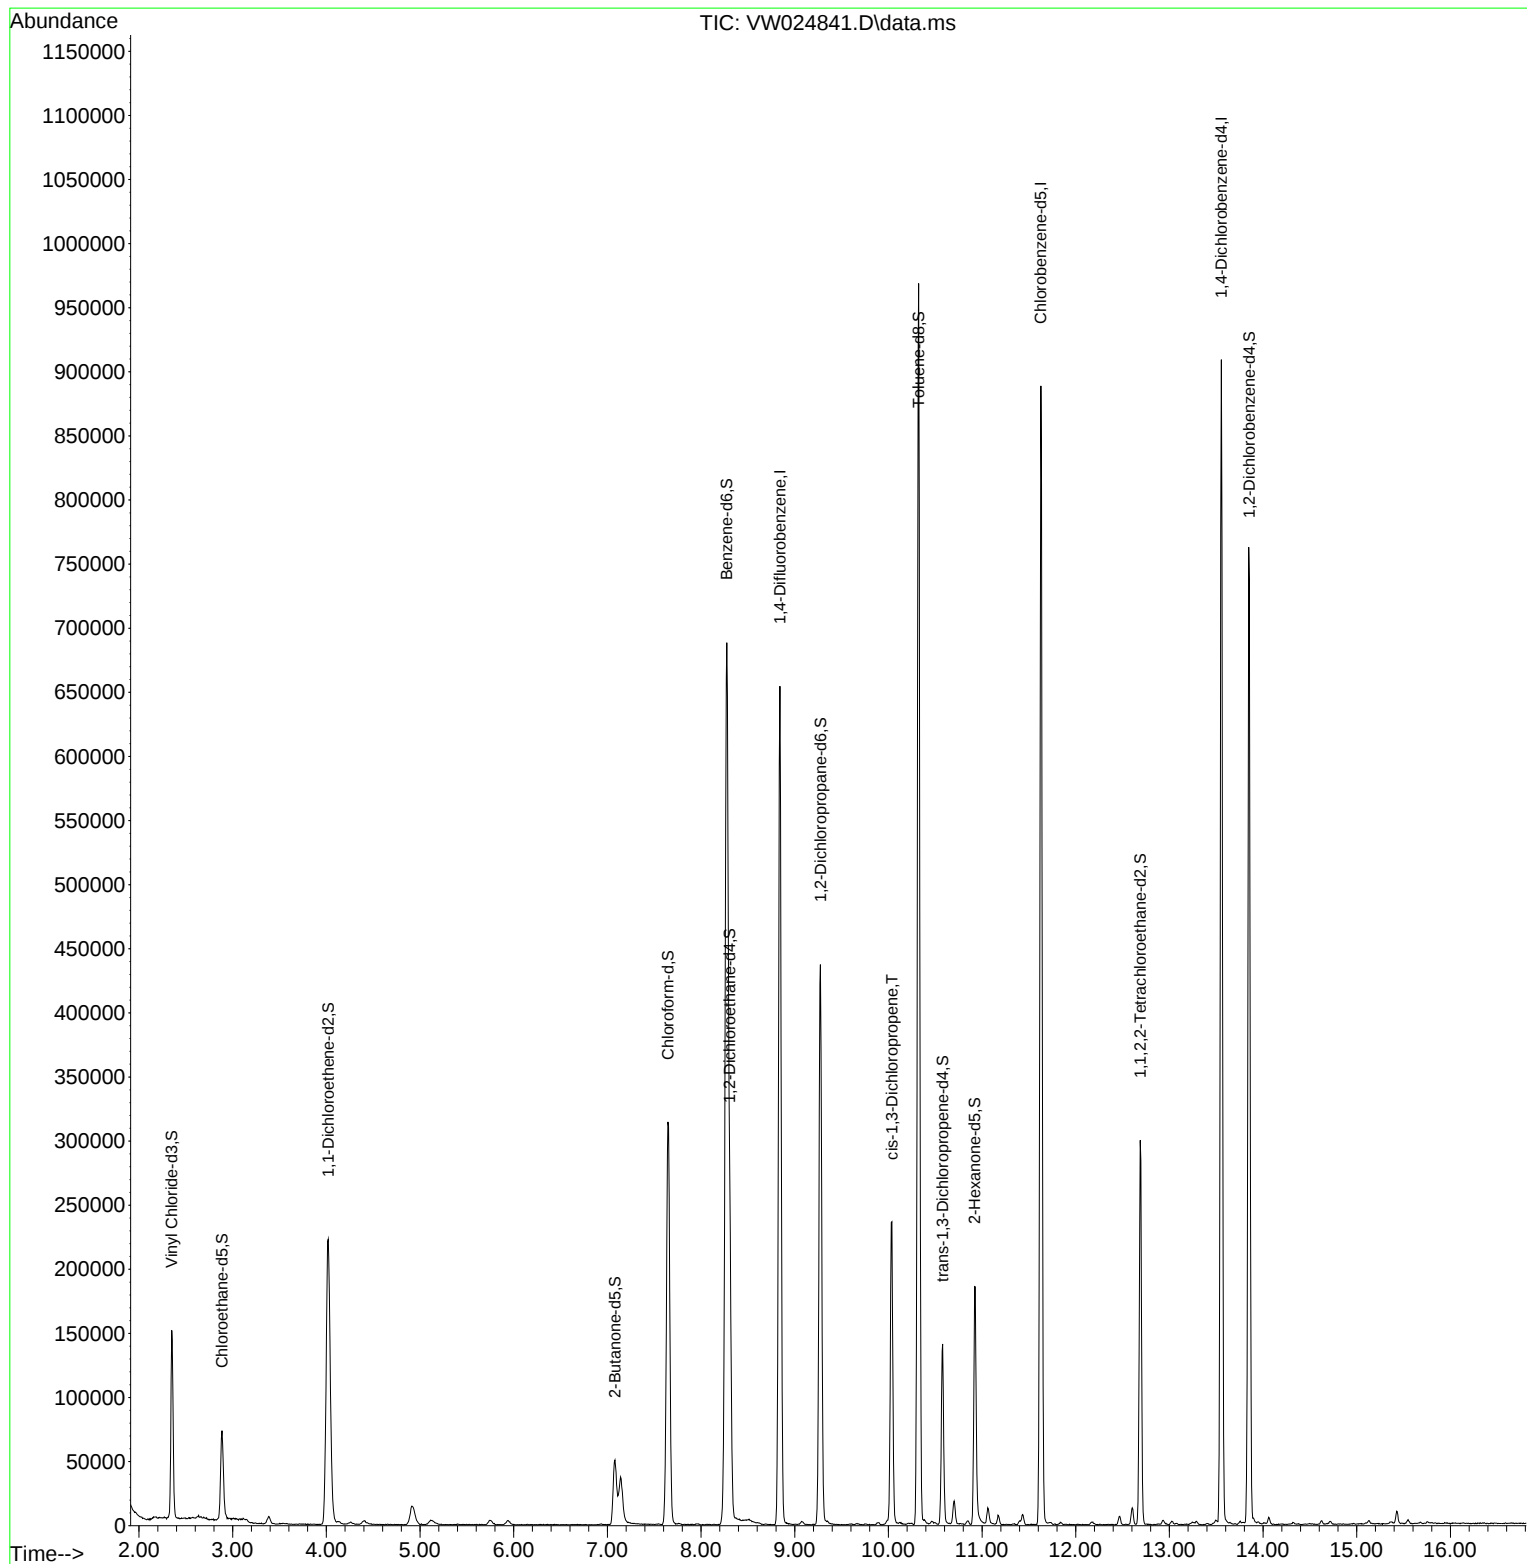

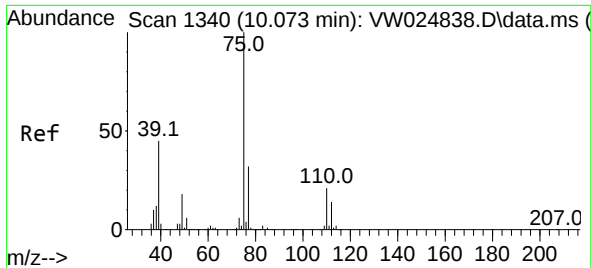

#39
 cis-1,3-Dichloropropene
 Concen: 0.475 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024841.D
 Acq: 11 Oct 2022 11:15

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion: 75 Resp: 6225
 Ion Ratio Lower Upper
 75 100
 77 46.7 22.4 41.6#

