

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
 Data File : VW024848.D
 Acq On : 11 Oct 2022 14:04
 Operator : SY/VA
 Sample : N5064-16
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COBN5

Quant Time: Oct 12 01:20:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	390622	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	352583	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156290	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	85114	20.826	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.320%
7) Chloroethane-d5	2.885	69	55030	23.171	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.680%
11) 1,1-Dichloroethene-d2	4.019	63	151260	15.991	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.960%
21) 2-Butanone-d5	7.080	46	109292	74.381	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	148.760%#
24) Chloroform-d	7.653	84	260850	24.979	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.920%
26) 1,2-Dichloroethane-d4	8.390	65	297	0.055	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	500177	22.195	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.760%
36) 1,2-Dichloropropane-d6	9.274	67	172817	25.099	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.400%
41) Toluene-d8	10.323	98	423711	21.036	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.160%
43) trans-1,3-Dichloroprop...	10.579	79	62915	20.518	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.080%
47) 2-Hexanone-d5	10.927	63	79847	67.777	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	135.560%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	168829	34.412	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	137.640%#
66) 1,2-Dichlorobenzene-d4	13.853	152	134648	24.483	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.920%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	12518	2.001	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024848.D
Acq On : 11 Oct 2022 14:04
Operator : SY/VA
Sample : N5064-16
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BN5

Quant Time: Oct 12 01:20:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

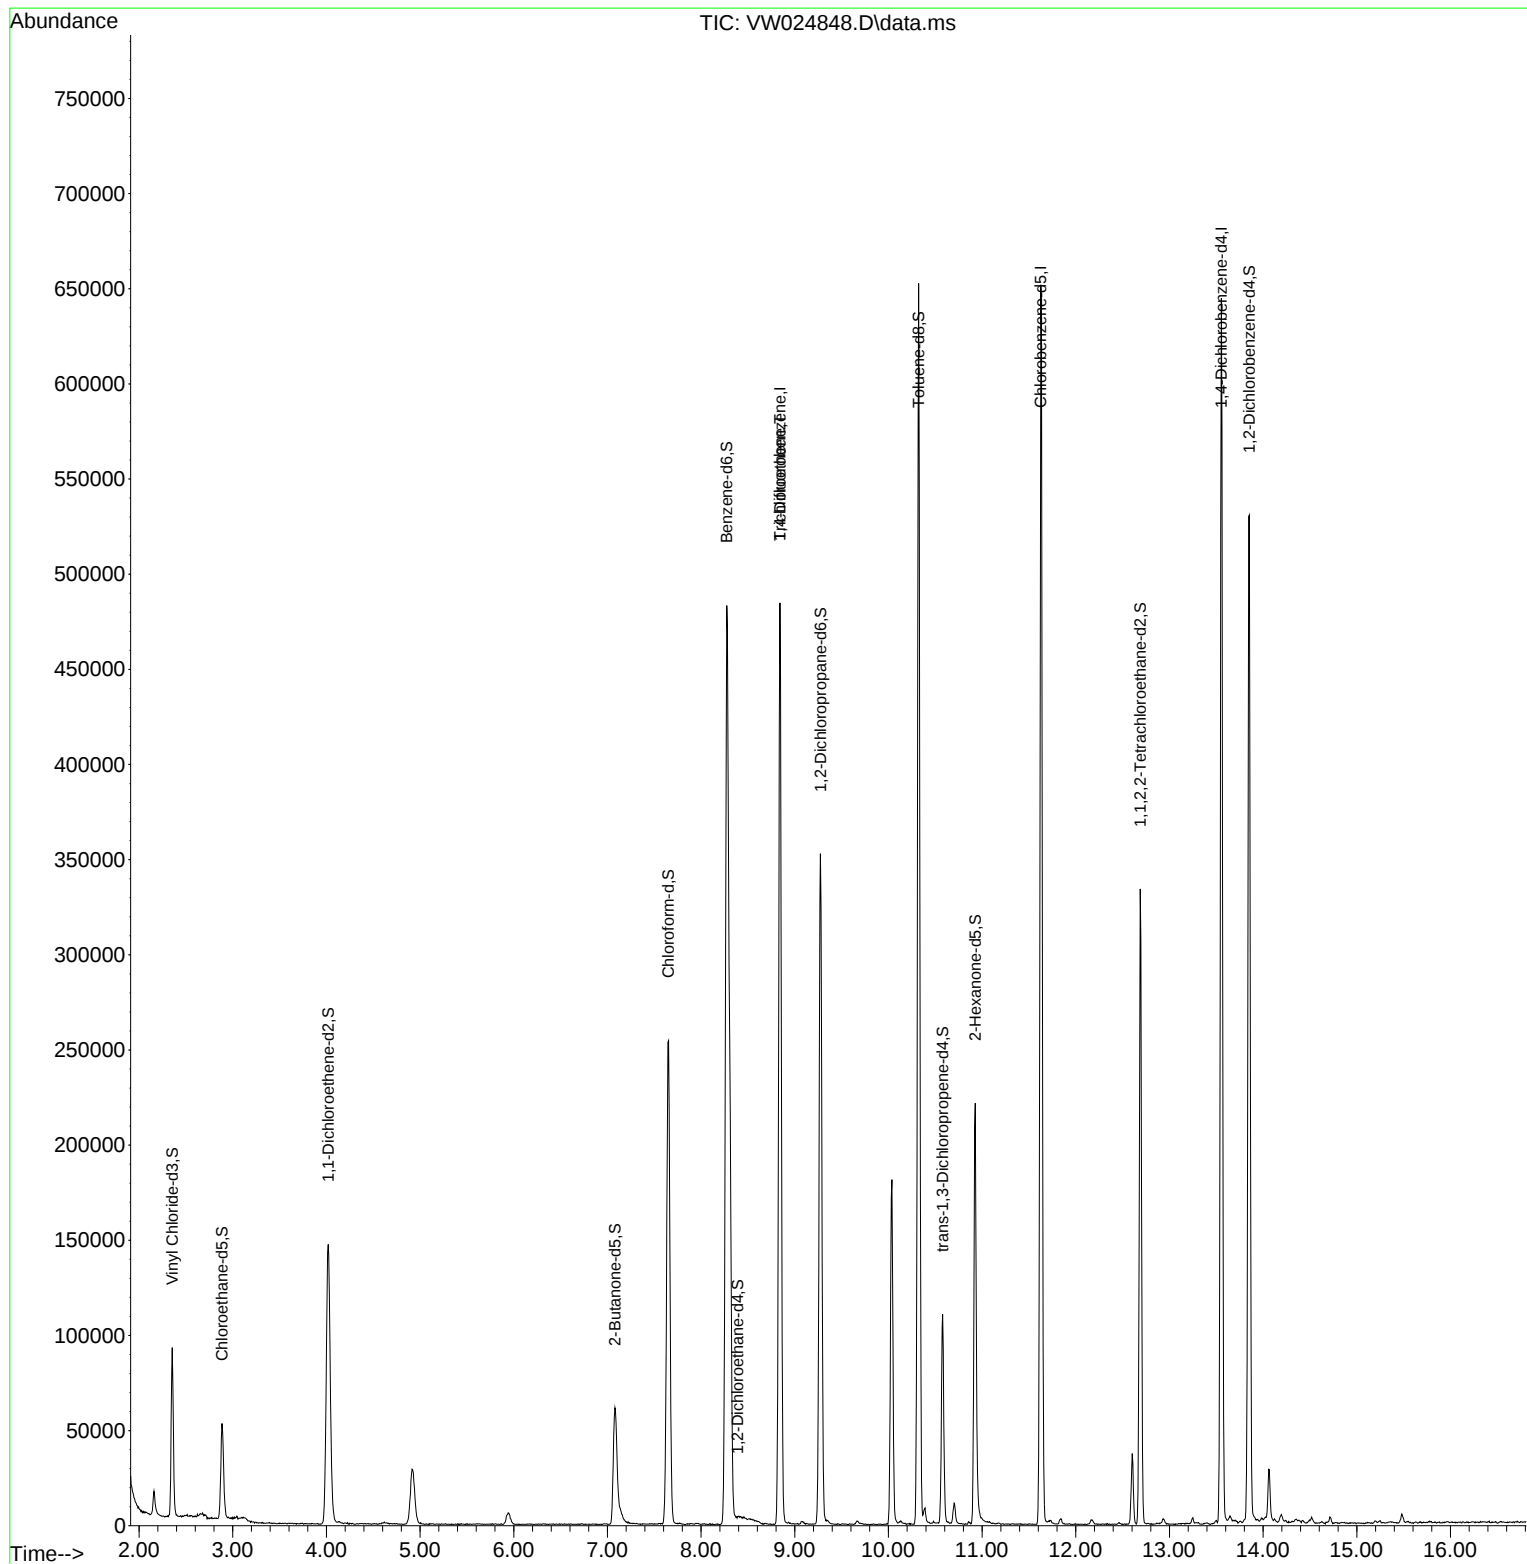

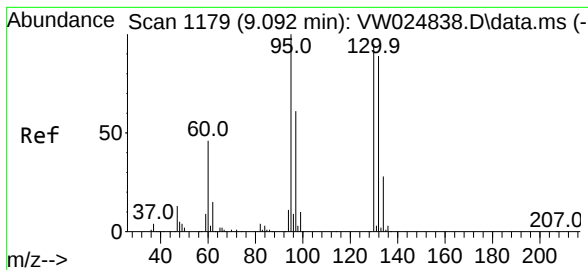

#34

Trichloroethene

Concen: 2.001 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW024848.D


Acq: 11 Oct 2022 14:04

Instrument :

MSVOA_W

ClientSampleId :

C0BN5

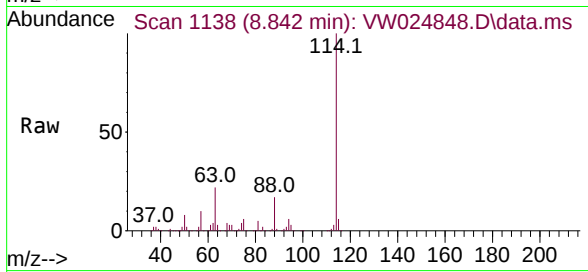

Tgt Ion: 95 Resp: 12518

Ion Ratio Lower Upper

95 100

97 0.0 43.5 80.9#

132 0.0 61.2 113.8#

130 0.0 68.5 127.1#

