

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
 Data File : VW024850.D
 Acq On : 11 Oct 2022 14:52
 Operator : SY/VA
 Sample : N5064-18
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COBN7

Quant Time: Oct 12 01:21:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	396666	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	343418	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	138340	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	86696	20.890	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.560%
7) Chloroethane-d5	2.885	69	58493	24.254	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	4.013	63	148292	15.438	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.760%
21) 2-Butanone-d5	7.086	46	80840	54.179	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.360%
24) Chloroform-d	7.653	84	238648	22.505	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	8.305	65	135660	24.661	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.640%
32) Benzene-d6	8.274	84	459864	20.950	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.800%
36) 1,2-Dichloropropane-d6	9.274	67	153709	22.919	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.680%
41) Toluene-d8	10.323	98	370990	18.910	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.640%
43) trans-1,3-Dichloroprop...	10.579	79	49764	16.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.640%
47) 2-Hexanone-d5	10.926	63	58986	51.405	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.820%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	135074	28.267	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.080%
66) 1,2-Dichlorobenzene-d4	13.847	152	110450	22.689	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.760%
Target Compounds						Qvalue
34) Trichloroethene	8.835	95	12063	1.980	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024850.D
Acq On : 11 Oct 2022 14:52
Operator : SY/VA
Sample : N5064-18
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BN7


Quant Time: Oct 12 01:21:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

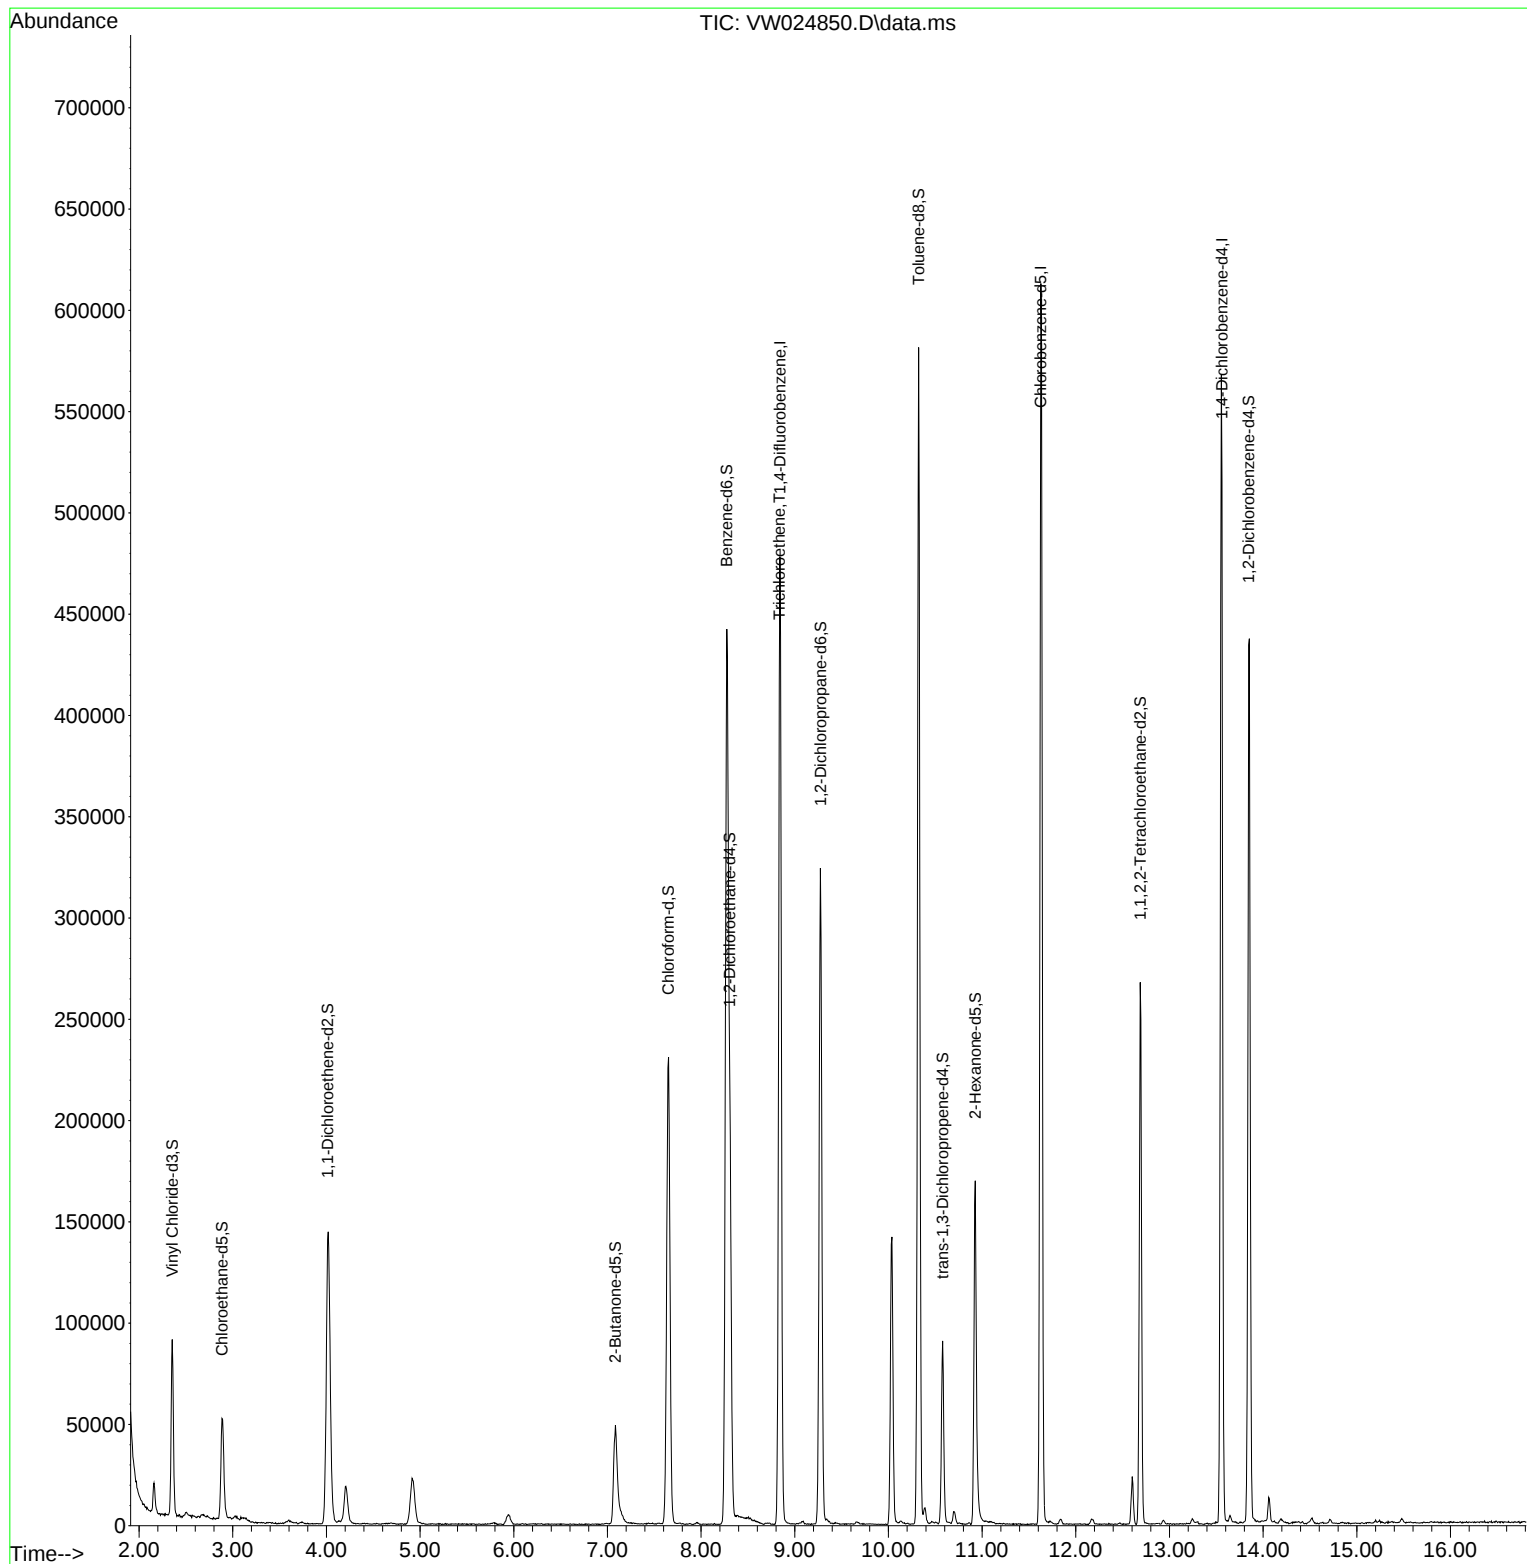

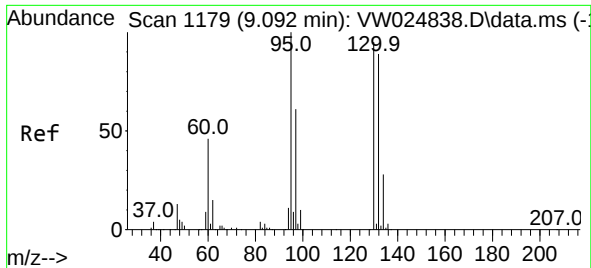

#34
 Trichloroethene
 Concen: 1.980 ug/L
 RT: 8.835 min Scan# 11
 Delta R.T. -0.256 min
 Lab File: VW024850.D
 Acq: 11 Oct 2022 14:52

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BN7

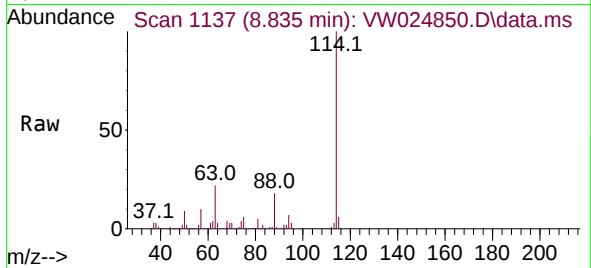

Tgt Ion:	95	Resp:	12063
Ion	Ratio	Lower	Upper
95	100		
97	0.0	43.5	80.9#
132	0.0	61.2	113.8#
130	0.0	68.5	127.1#

