

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
 Data File : VW024855.D
 Acq On : 11 Oct 2022 16:52
 Operator : SY/VA
 Sample : N5049-06RE
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BJ6

Quant Time: Oct 12 01:22:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	557527	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	467286	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	200325	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	121645	20.854	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.400%
7) Chloroethane-d5	2.885	69	76637	22.609	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.440%
11) 1,1-Dichloroethene-d2	4.019	63	205446	15.217	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.880%
21) 2-Butanone-d5	7.086	46	106478	50.772	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.540%
24) Chloroform-d	7.647	84	353548	23.721	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.880%
26) 1,2-Dichloroethane-d4	8.305	65	189575	24.519	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.080%
32) Benzene-d6	8.275	84	684626	22.922	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.680%
36) 1,2-Dichloropropane-d6	9.274	67	226104	24.777	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.120%
41) Toluene-d8	10.323	98	572394	21.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.760%
43) trans-1,3-Dichloroprop...	10.579	79	70754	17.410	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.640%
47) 2-Hexanone-d5	10.927	63	73707	47.207	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.420%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	181075	27.848	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	158406	22.471	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.880%
Target Compounds					Qvalue	
48) 2-Hexanone	10.920	43	10391	3.215	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024855.D
Acq On : 11 Oct 2022 16:52
Operator : SY/VA
Sample : N5049-06RE
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BJ6


Quant Time: Oct 12 01:22:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

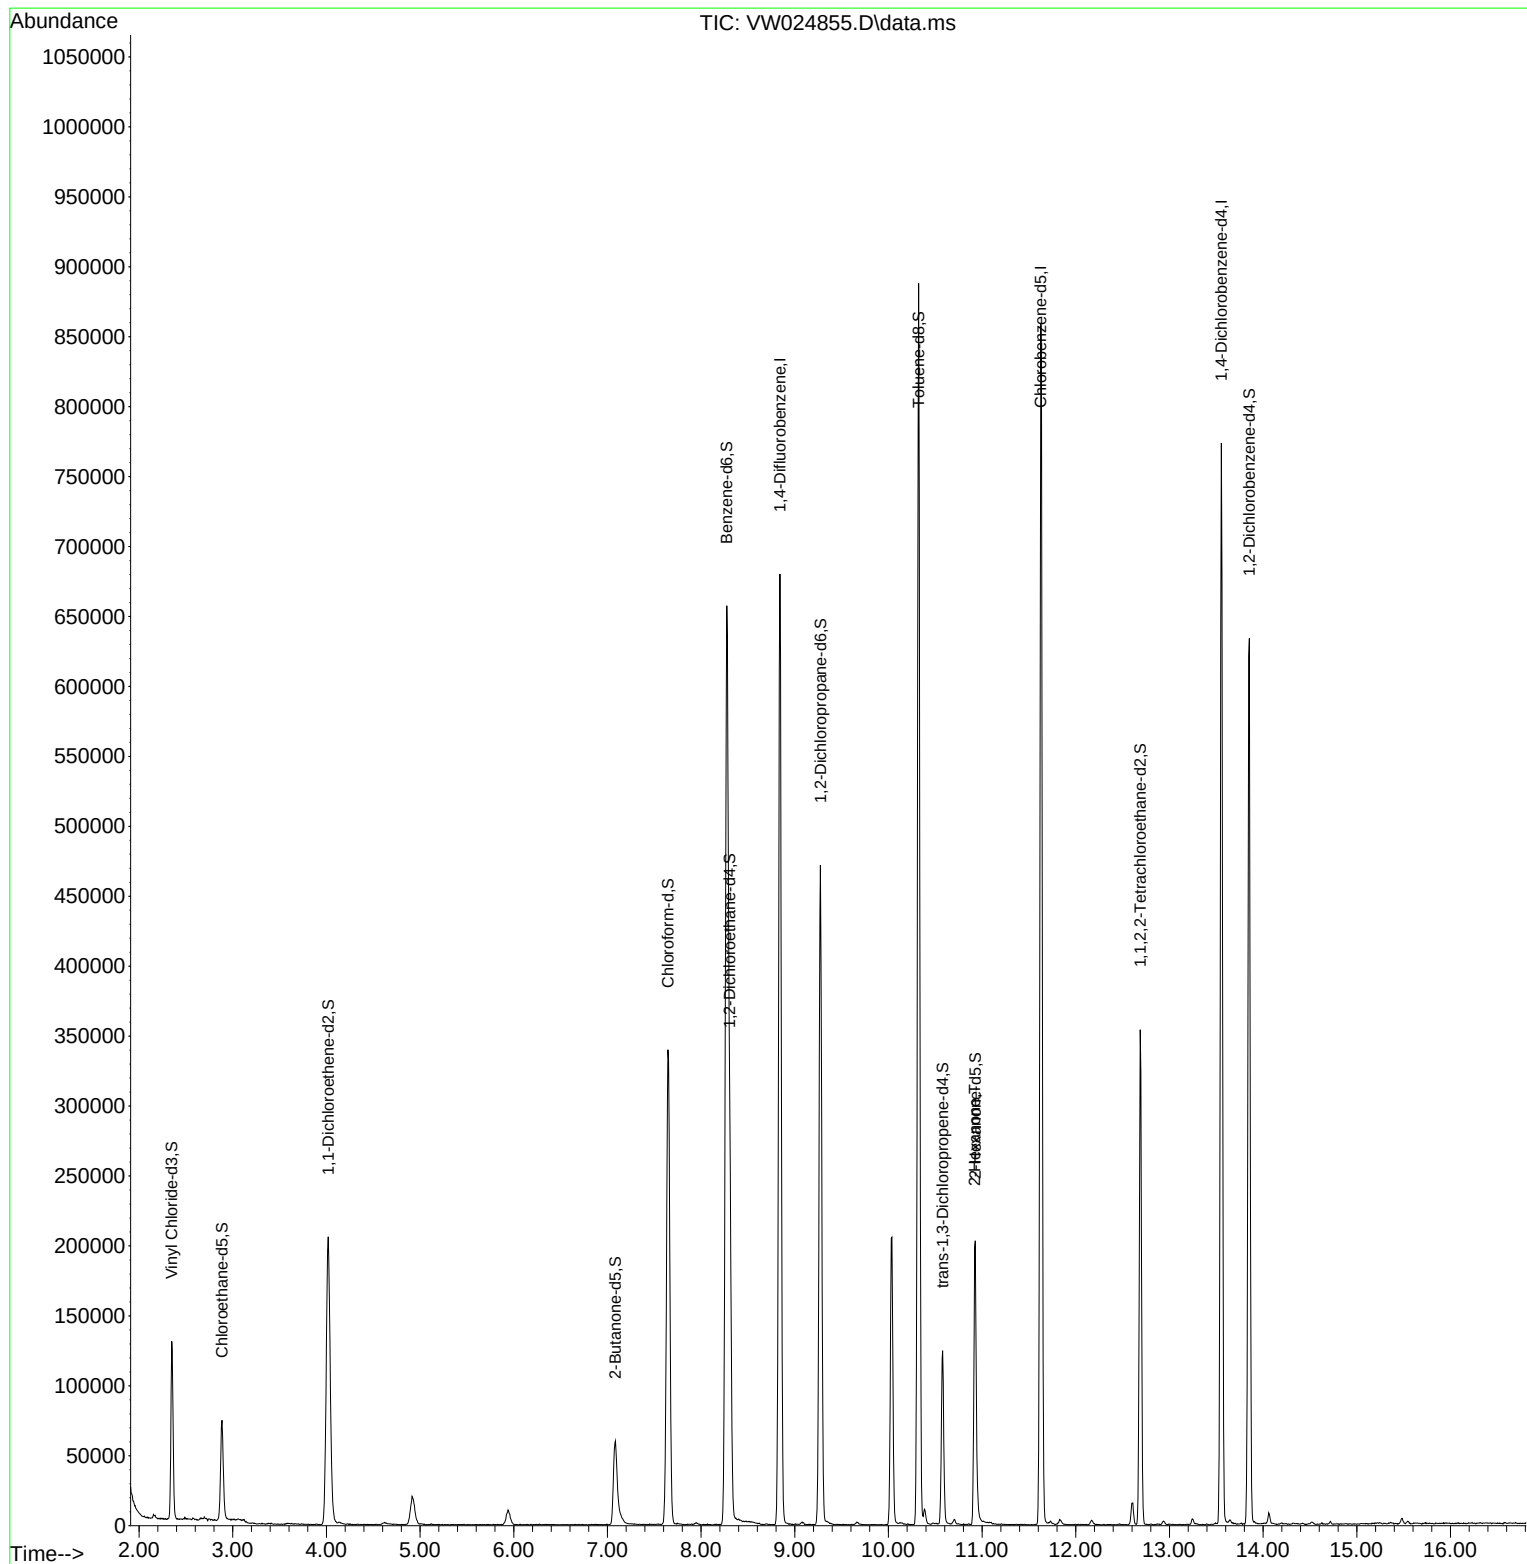

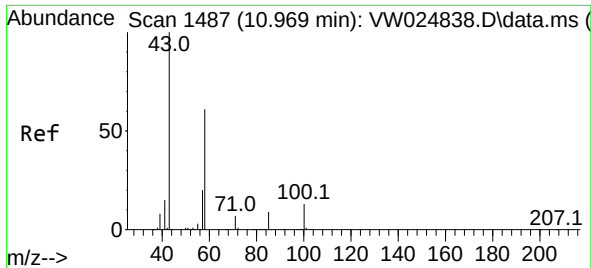

#48
 2-Hexanone
 Concen: 3.215 ug/L
 RT: 10.920 min Scan# 14
 Delta R.T. -0.049 min
 Lab File: VW024855.D
 Acq: 11 Oct 2022 16:52

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BJ6

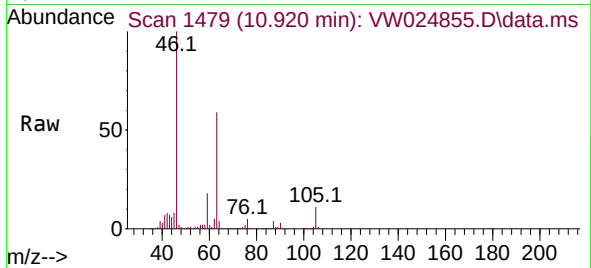

Tgt Ion: 43 Resp: 10391
 Ion Ratio Lower Upper
 43 100
 58 21.3 45.3 67.9#
 57 20.0 16.3 24.5
 100 1.1 10.4 15.6#

