




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024860.D
Acq On : 11 Oct 2022 18:53
Operator : SY/VA
Sample : N5049-11RE
Misc : 6.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 01:23:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

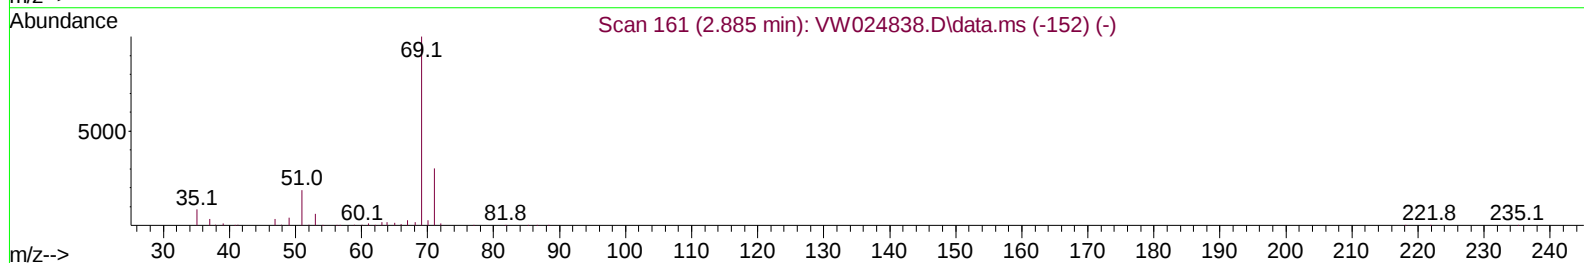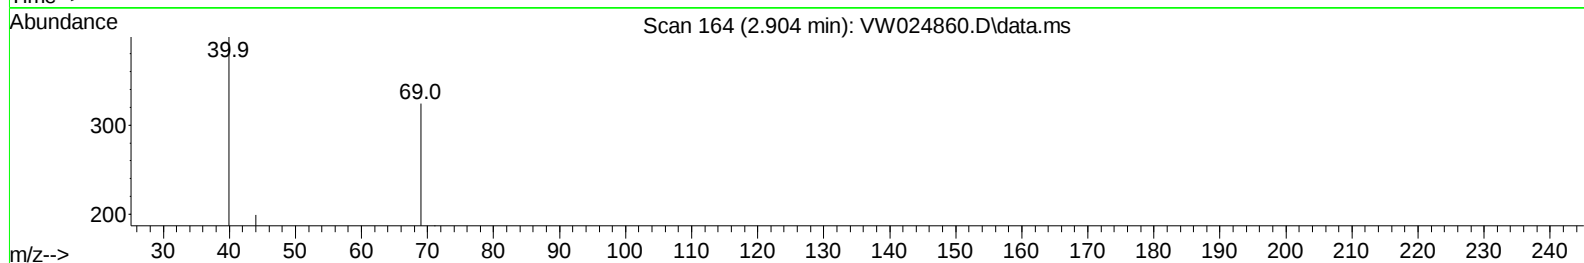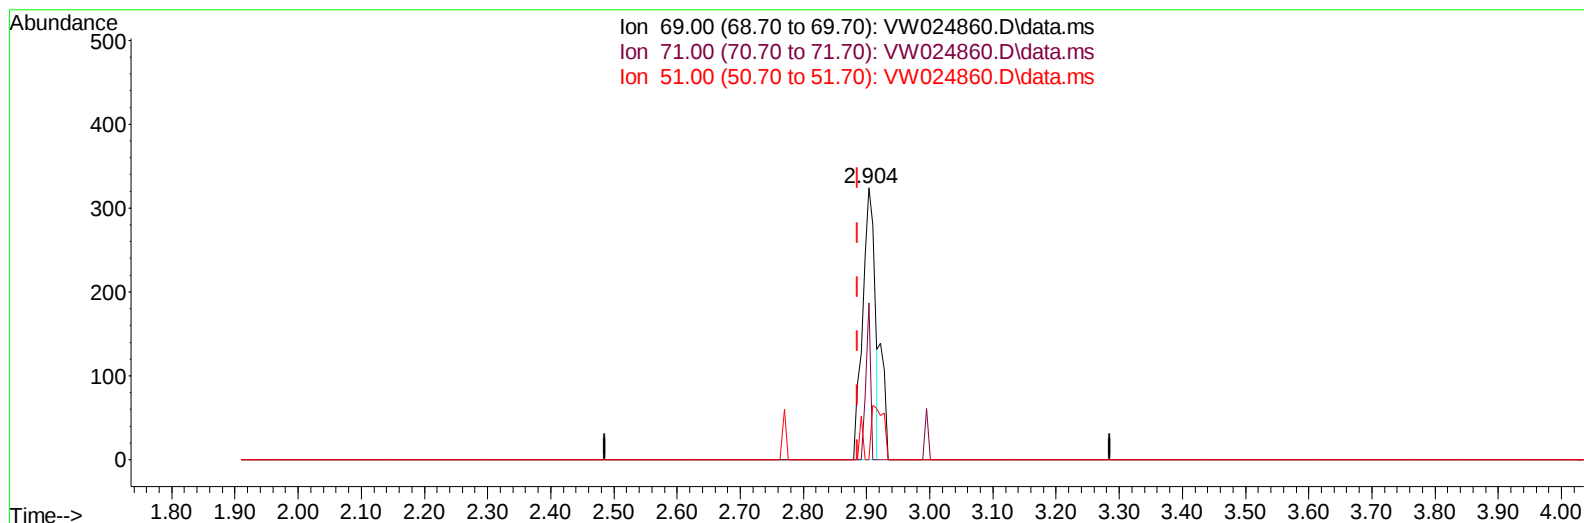

TIC: VW024860.D\data.ms

(7) Chloroethane-d5 (S)

2.904min (+ 0.018) 85.77 ug/L

response 437

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.20	21.97#
51.00	21.50	14.87#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
 Data File : VW024860.D
 Acq On : 11 Oct 2022 18:53
 Operator : SY/VA
 Sample : N5049-11RE
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP7RE

Manual IntegrationsAPPROVED

Quant Time: Oct 12 01:23:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

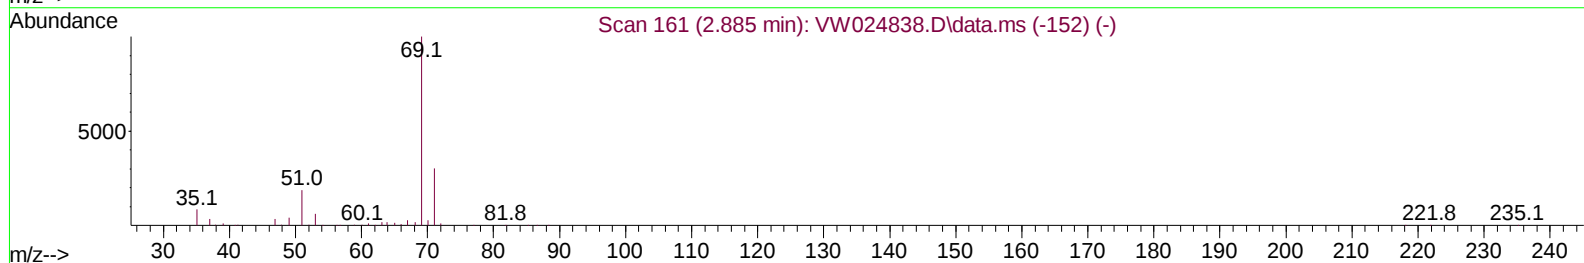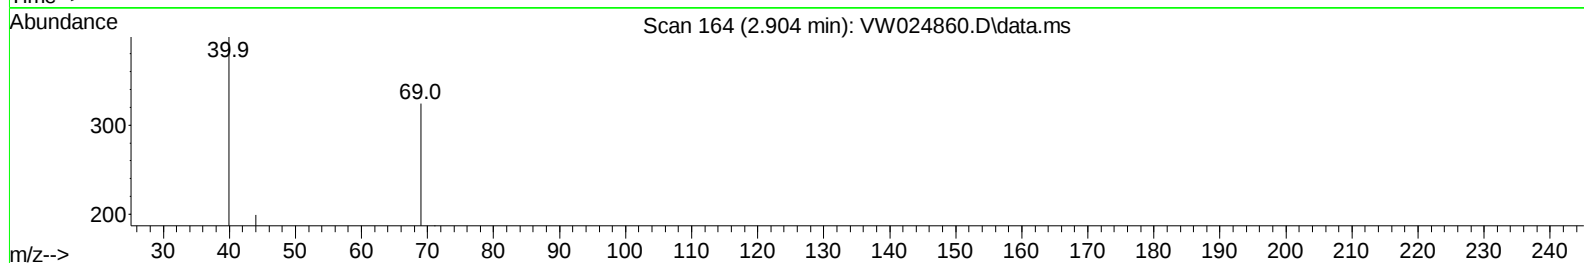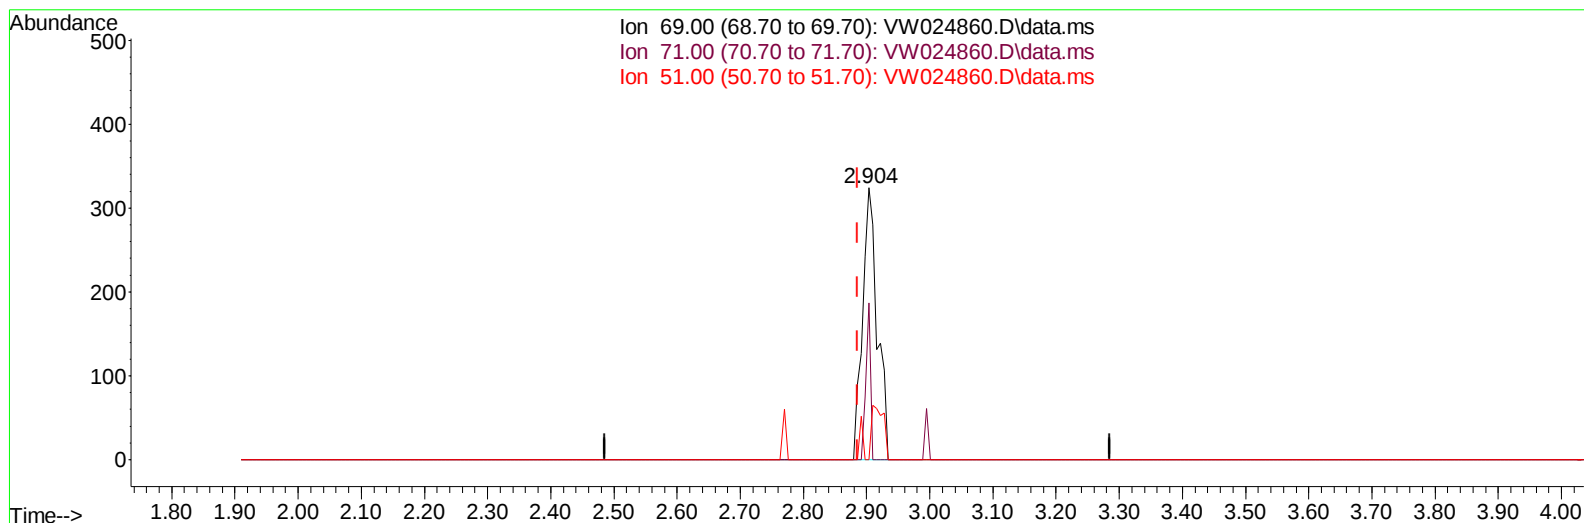

TIC: VW024860.D\data.ms

(7) Chloroethane-d5 (S)

2.904min (+ 0.018) 103.44 ug/L m

response 527

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.20	18.22#
51.00	21.50	12.33#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024860.D
Acq On : 11 Oct 2022 18:53
Operator : SY/VA
Sample : N5049-11RE
Misc : 6.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 01:23:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

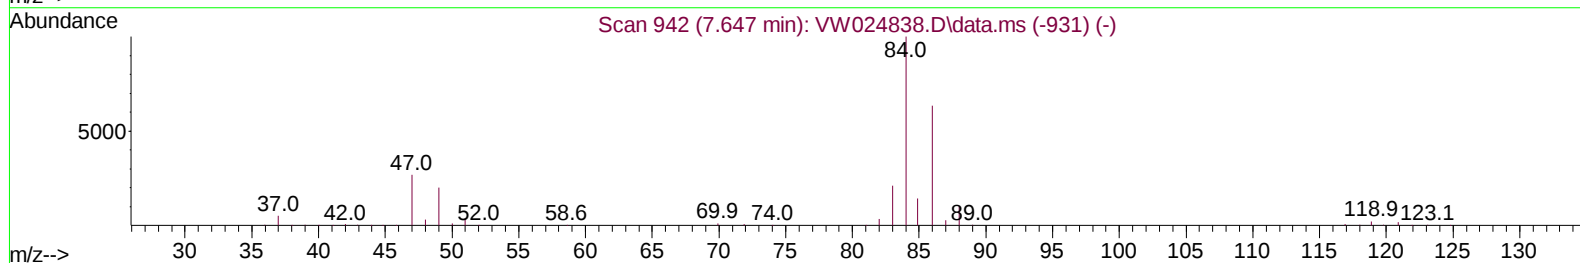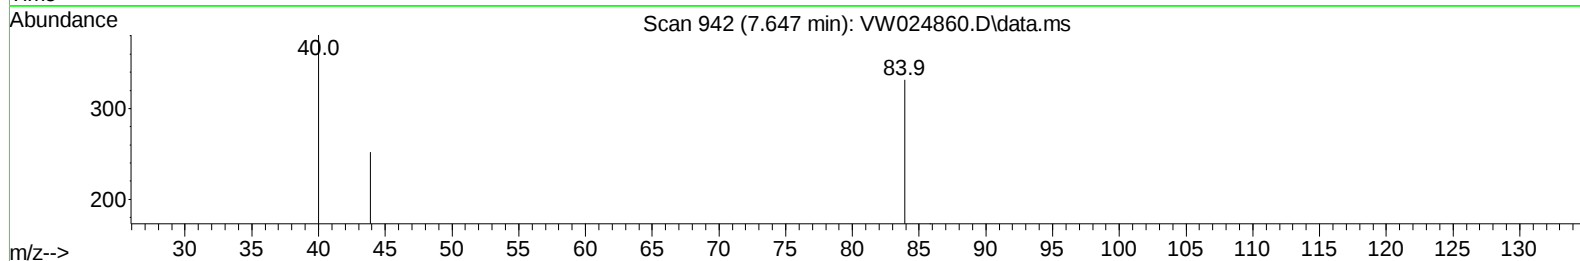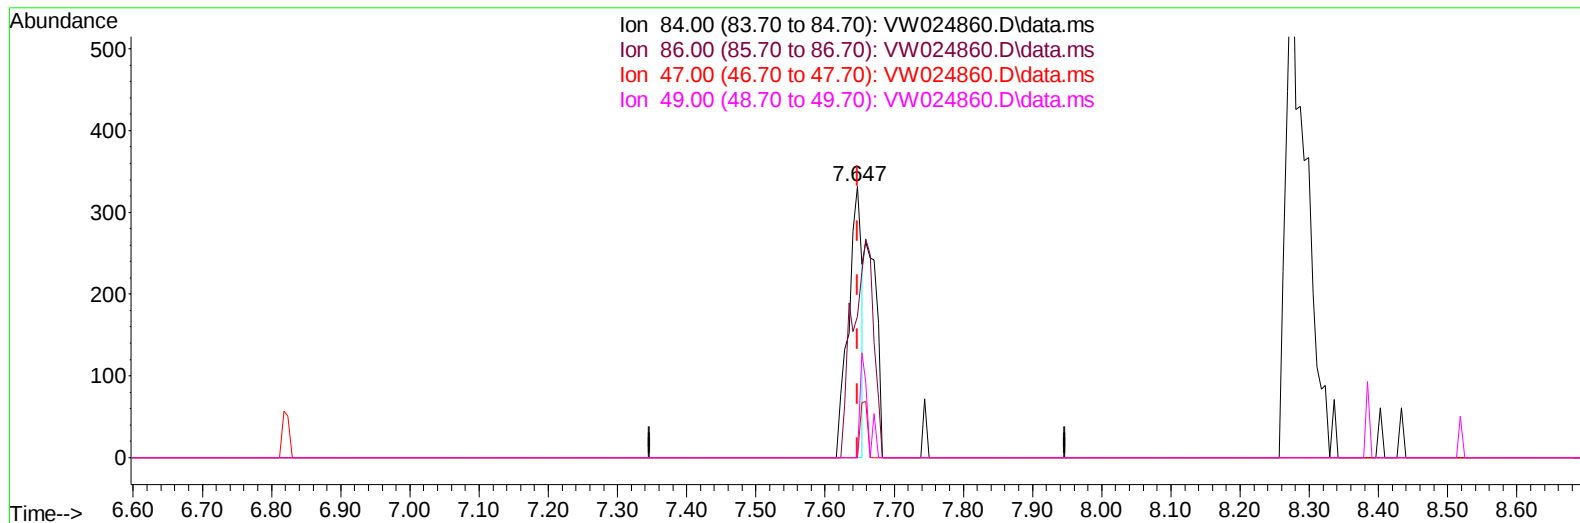

TIC: VW024860.D\data.ms

(24) Chloroform-d (S)

7.647min (-0.000) 19.69 ug/L

response 441

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	93.65#
47.00	45.50	11.34#
49.00	25.90	18.14




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024860.D
Acq On : 11 Oct 2022 18:53
Operator : SY/VA
Sample : N5049-11RE
Misc : 6.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 01:23:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

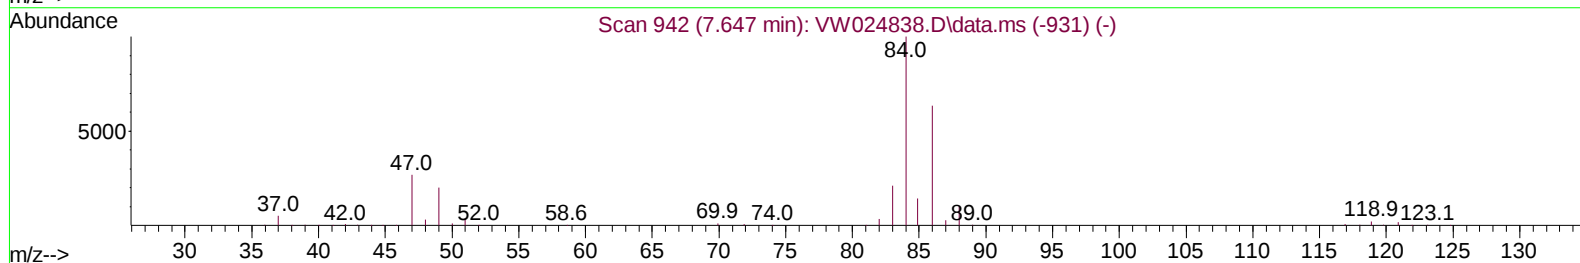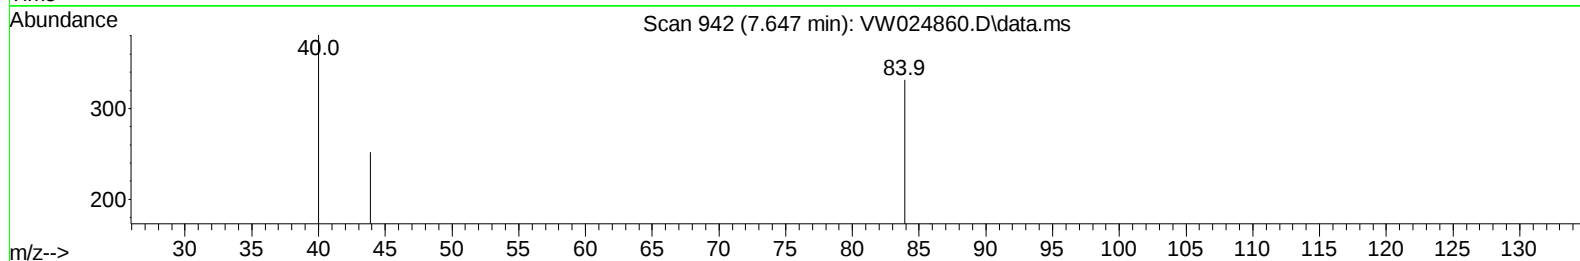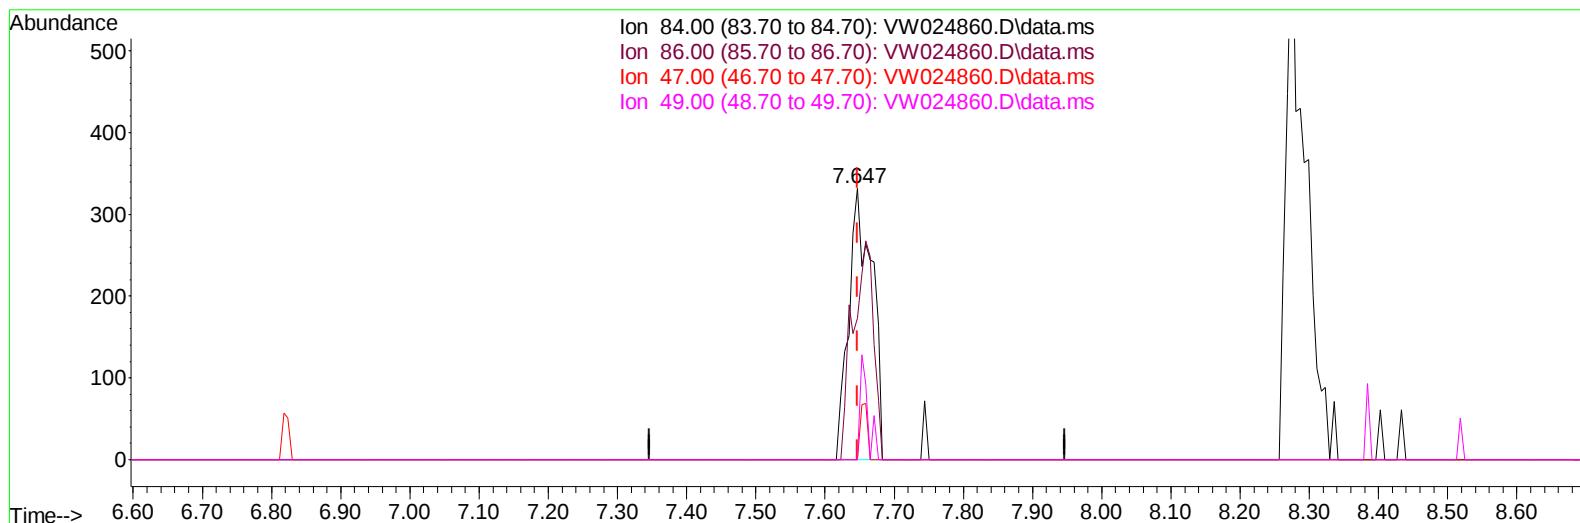

TIC: VW024860.D\data.ms

(24) Chloroform-d (S)

7.647min (-0.000) 34.64 ug/L m

response 776

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.50	53.22
47.00	45.50	6.44#
49.00	25.90	10.31#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101122\
 Data File : VW024860.D
 Acq On : 11 Oct 2022 18:53
 Operator : SY/VA
 Sample : N5049-11RE
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 01:23:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 01:17:56 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.854	114		838	25.000	ug/L	# 0.01
28) Chlorobenzene-d5	11.634	117		506	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	0.000	152		0	0.000	ug/L	-13.55
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.361	65		595	67.863	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	271.440%#	
7) Chloroethane-d5	2.904	69		527m	103.435	ug/L	0.02
Spiked Amount 25.000	Range 30	- 150		Recovery	=	413.760%#	
11) 1,1-Dichloroethene-d2	4.031	63		808	39.816	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	159.280%#	
21) 2-Butanone-d5	0.000	46		0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery	=	0.000%#	
24) Chloroform-d	7.647	84		776m	34.639	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	138.560%	
26) 1,2-Dichloroethane-d4	8.311	65		269	23.147	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	92.600%	
32) Benzene-d6	8.275	84		1213	37.506	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	150.040%#	
36) 1,2-Dichloropropane-d6	9.268	67		404	40.884	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	163.520%#	
41) Toluene-d8	10.323	98		889	30.755	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	123.000%	
43) trans-1,3-Dichloroprop...	0.000	79		0d	0.000	ug/L	
Spiked Amount 25.000	Range 30	- 135		Recovery	=	0.000%#	
47) 2-Hexanone-d5	0.000	63		0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135		Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.701	84		207	29.400	ug/L	0.01
Spiked Amount 25.000	Range 45	- 120		Recovery	=	117.600%	
66) 1,2-Dichlorobenzene-d4	0.000	152		0	0.000	ug/L	
Spiked Amount 25.000	Range 75	- 120		Recovery	=	0.000%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101122\
Data File : VW024860.D
Acq On : 11 Oct 2022 18:53
Operator : SY/VA
Sample : N5049-11RE
Misc : 6.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

Quant Time: Oct 12 01:23:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 01:17:56 2022
Response via : Initial Calibration

