

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030555.D
 Acq On : 11 Oct 2024 17:38
 Operator : SY/MD
 Sample : P4350-04
 Misc : 5.97g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 14 01:43:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 01:34:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	599823	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	544489	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	245823	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	185430	19.667	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.680%
7) Chloroethane-d5	2.899	69	148317	20.782	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.120%
11) 1,1-Dichloroethene-d2	4.021	65	79268	20.214	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.840%
21) 2-Butanone-d5	7.075	46	79648	46.942	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.880%
24) Chloroform-d	7.648	84	351400	20.485	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.960%
26) 1,2-Dichloroethane-d4	8.306	65	210051	23.548	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	8.270	84	658755	20.845	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.400%
36) 1,2-Dichloropropane-d6	9.270	67	206750	22.290	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.160%
41) Toluene-d8	10.324	98	587306	20.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.440%
43) trans-1,3-Dichloroprop...	10.574	79	86747	22.335	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.320%
47) 2-Hexanone-d5	10.922	63	65052	54.451	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	164715	24.180	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	195419	23.495	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.960%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	7401	0.554	ug/L	Qvalue # 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030555.D
Acq On : 11 Oct 2024 17:38
Operator : SY/MD
Sample : P4350-04
Misc : 5.97g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 14 01:43:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 01:34:28 2024
Response via : Initial Calibration

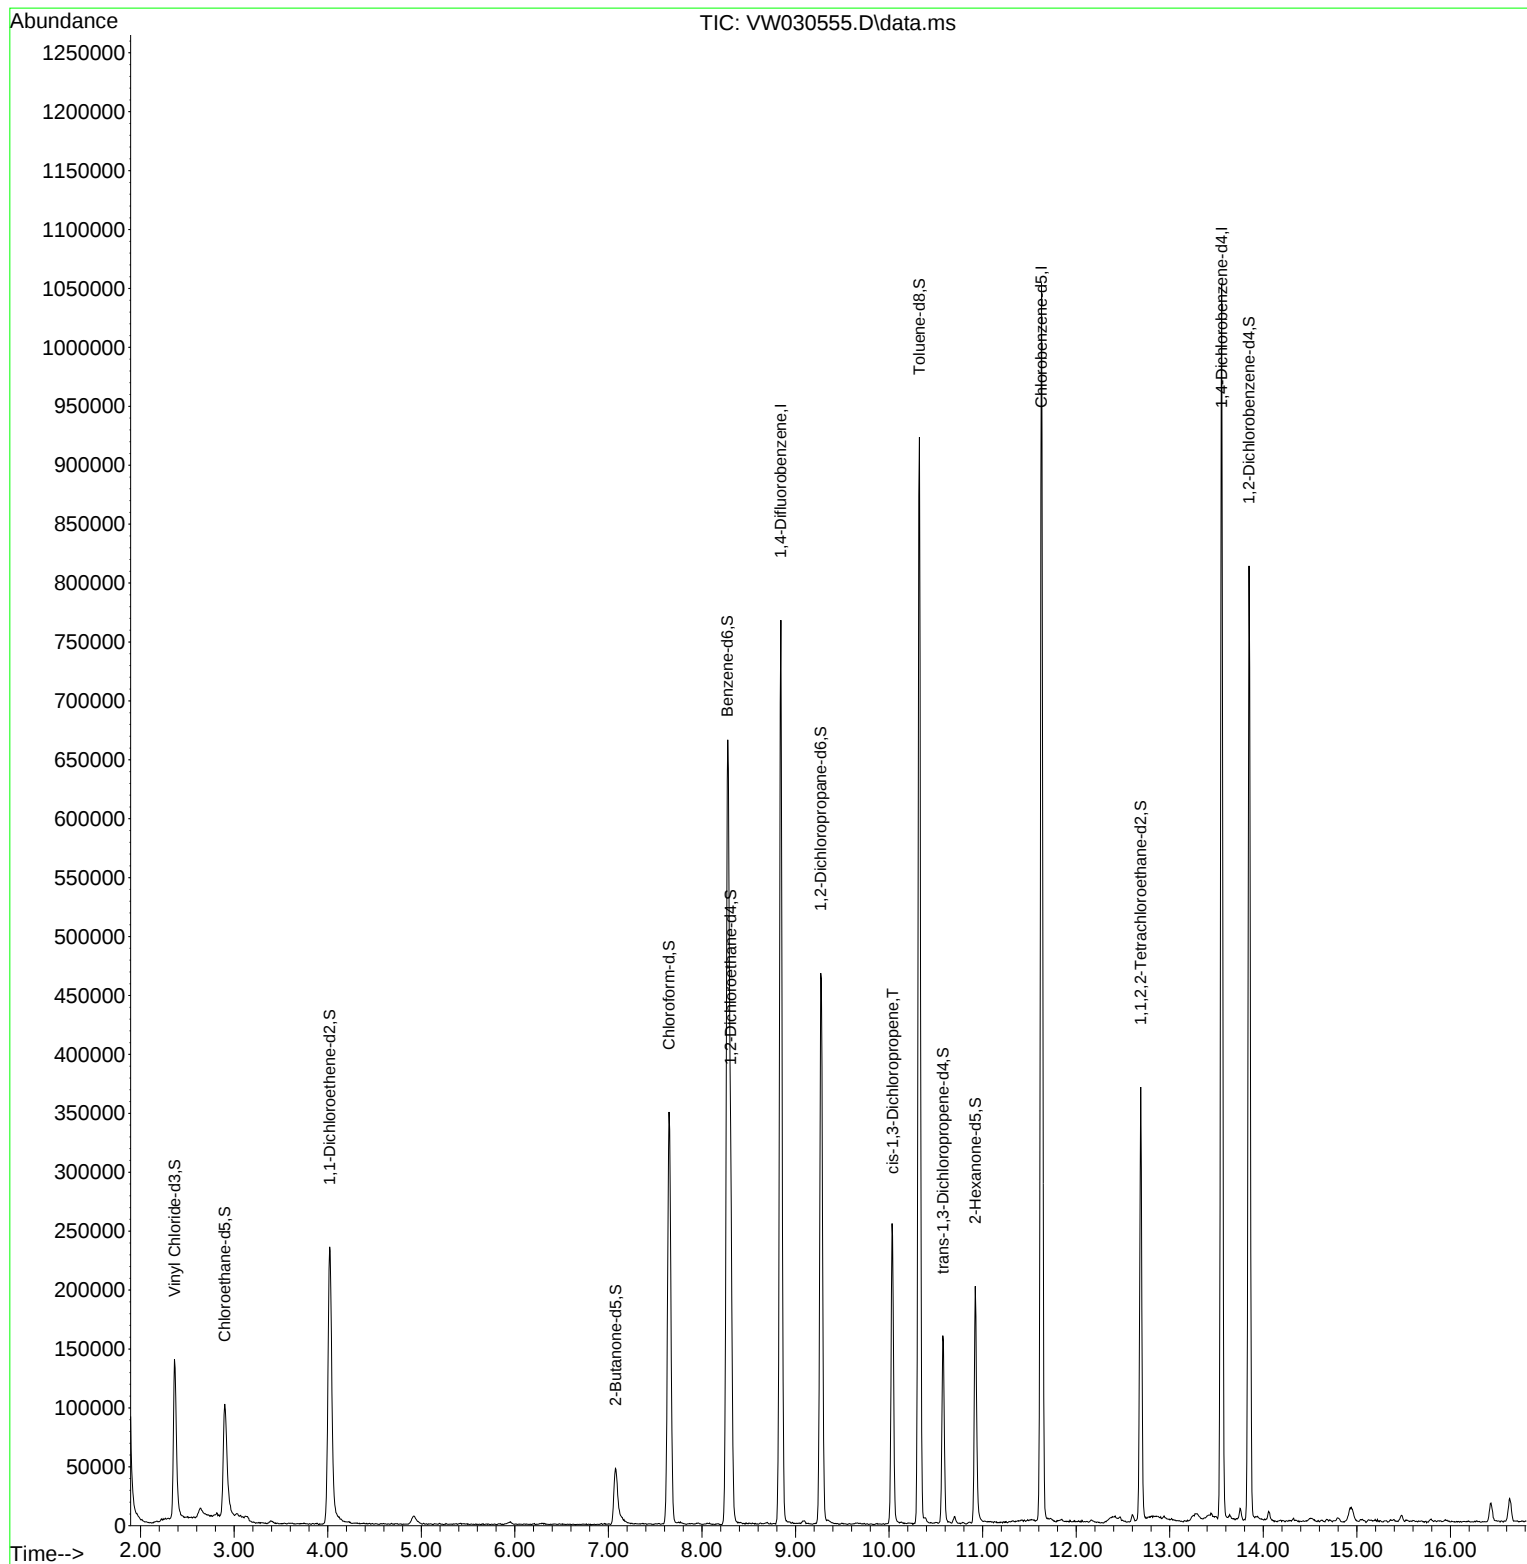

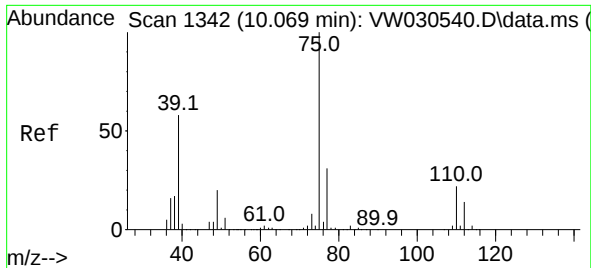

#39
 cis-1,3-Dichloropropene
 Concen: 0.554 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW030555.D
 Acq: 11 Oct 2024 17:38

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 7401
 Ion Ratio Lower Upper
 75 100
 77 43.1 21.1 39.1#

