

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030569.D
 Acq On : 12 Oct 2024 00:25
 Operator : SY/MD
 Sample : P4361-07
 Misc : 3.25g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 14 04:49:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	462219	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	348569	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	131123	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	181713	25.011	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.040%
7) Chloroethane-d5	2.899	69	146247	26.592	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.360%
11) 1,1-Dichloroethene-d2	4.021	65	72811	24.095	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	96.360%
21) 2-Butanone-d5	7.075	46	70046	53.573	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.140%
24) Chloroform-d	7.770	84	168	0.013	ug/L	0.12
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.040%#
26) 1,2-Dichloroethane-d4	8.307	65	179282	26.083	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.320%
32) Benzene-d6	8.276	84	601482	29.731	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	118.920%
36) 1,2-Dichloropropane-d6	9.270	67	180497	30.397	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	121.600%#
41) Toluene-d8	10.325	98	475925	25.770	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.080%
43) trans-1,3-Dichloroprop...	10.575	79	66568	26.773	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	107.080%
47) 2-Hexanone-d5	10.922	63	55517	72.590	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.180%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	126194	28.938	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	110686	24.948	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.800%
Target Compounds						Qvalue
13) Acetone	4.125	43	12095	6.319	ug/L	94
39) cis-1,3-Dichloropropene	10.032	75	5488	0.642	ug/L #	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030569.D
Acq On : 12 Oct 2024 00:25
Operator : SY/MD
Sample : P4361-07
Misc : 3.25g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 14 04:49:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration




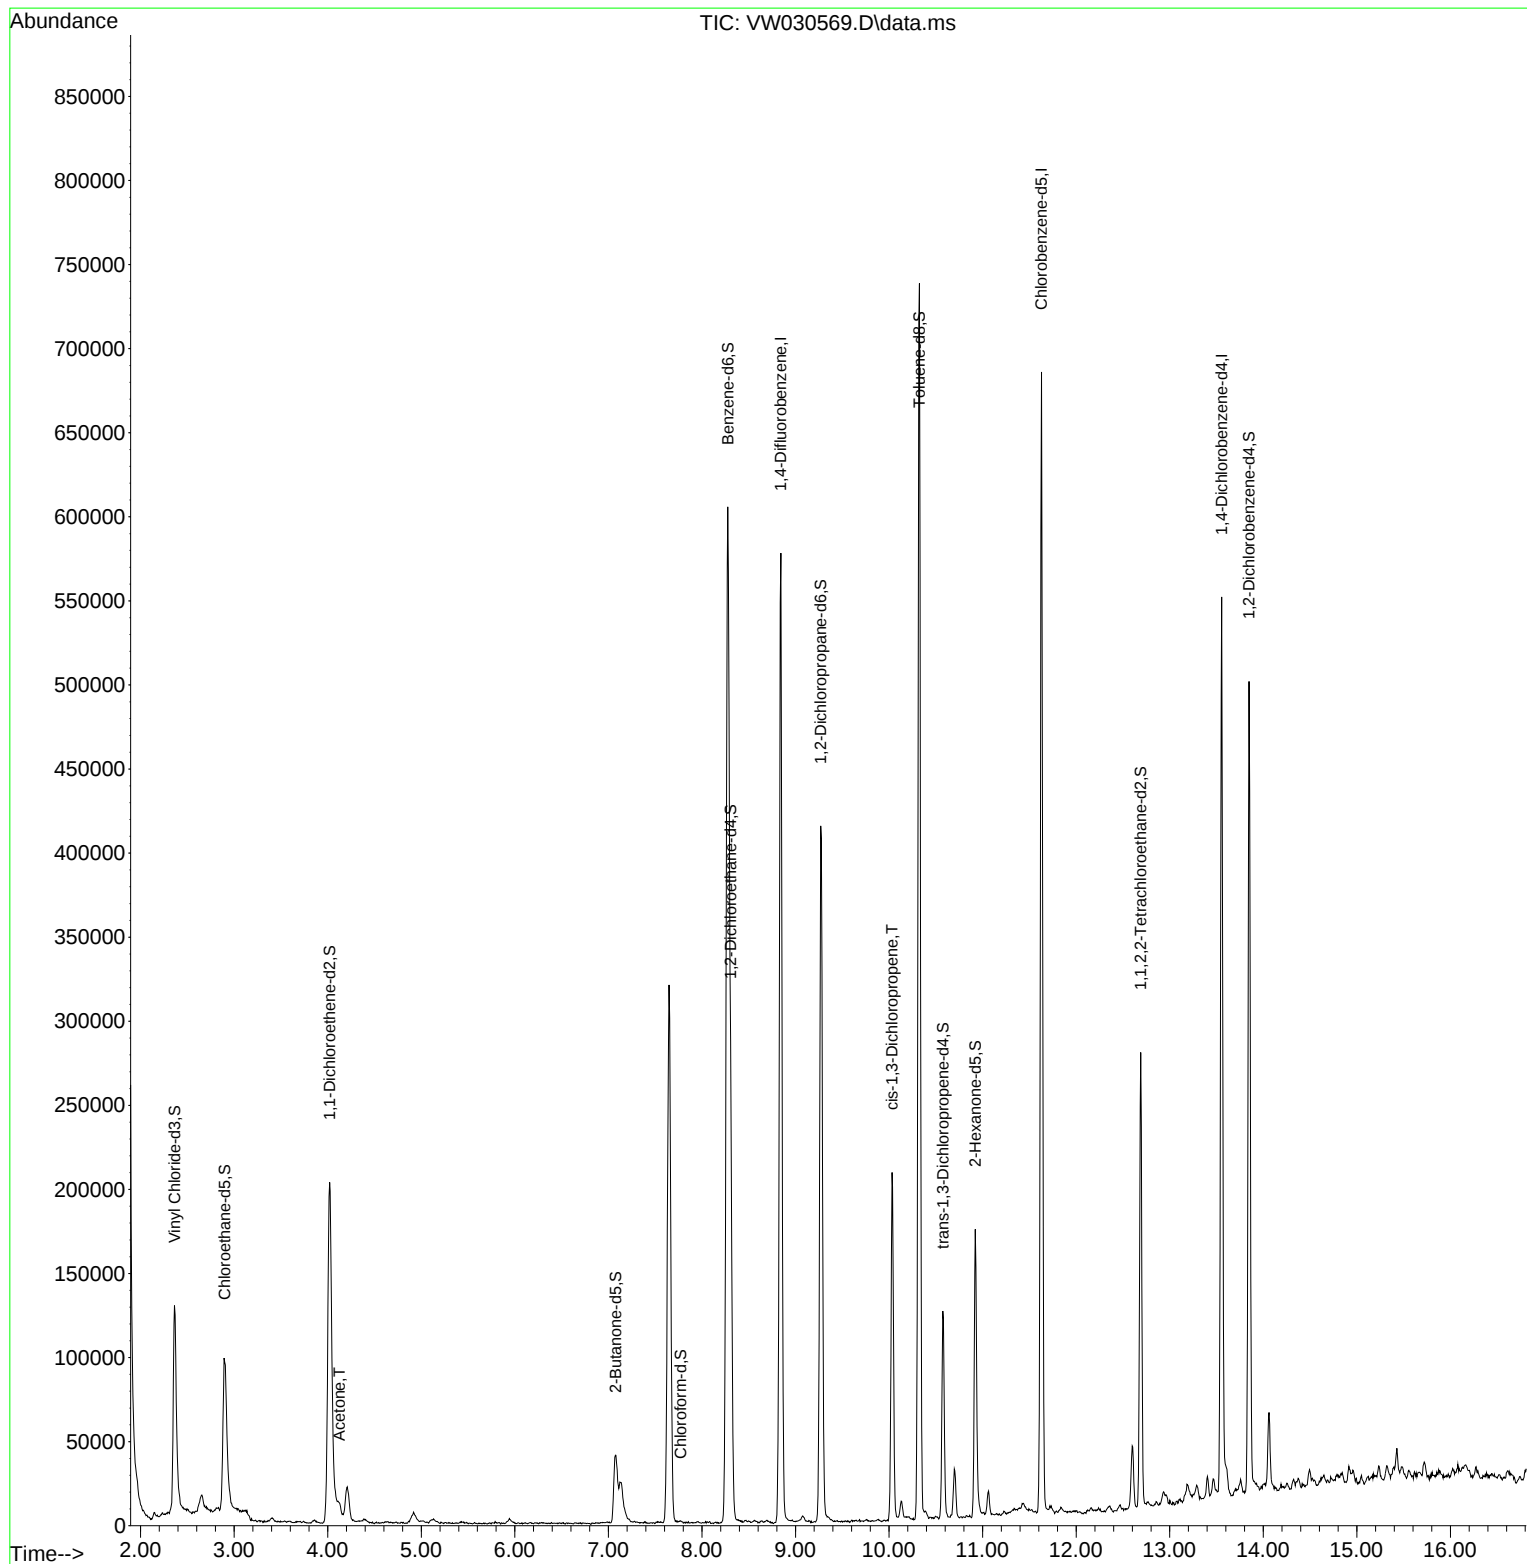


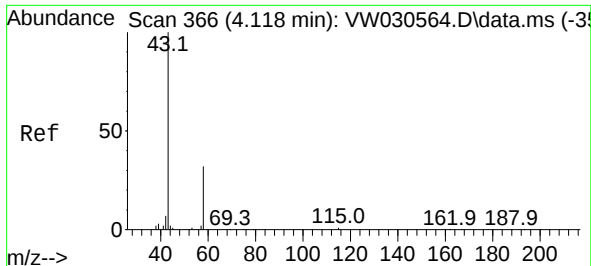

#13
Acetone
Concen: 6.319 ug/L
RT: 4.125 min Scan# 3
Delta R.T. 0.006 min
Lab File: VW030569.D
Acq: 12 Oct 2024 00:25

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 12095
Ion Ratio Lower Upper
43 100
58 31.8 0.0 57.6

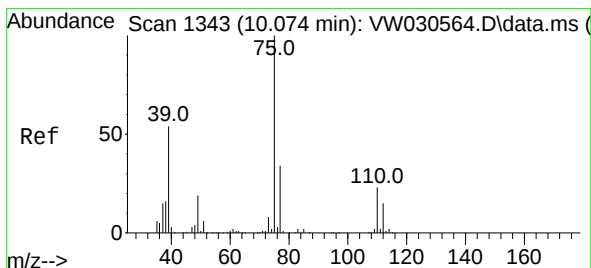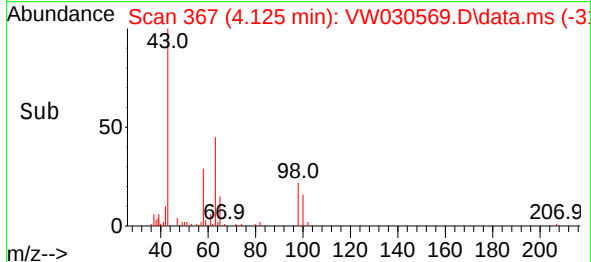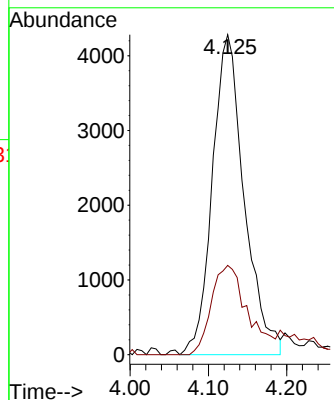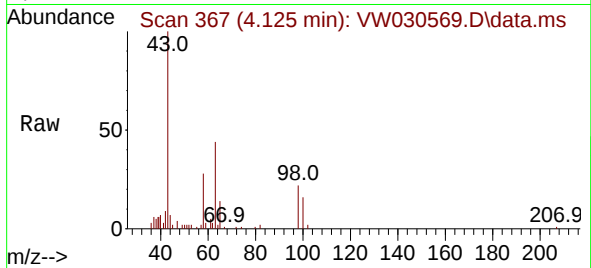

#39
cis-1,3-Dichloropropene
Concen: 0.642 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.042 min
Lab File: VW030569.D
Acq: 12 Oct 2024 00:25

Tgt Ion: 75 Resp: 5488
Ion Ratio Lower Upper
75 100
77 53.5 21.1 39.1#

