




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030569.D
Acq On : 12 Oct 2024 00:25
Operator : SY/MD
Sample : P4361-07
Misc : 3.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAY9

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:49:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

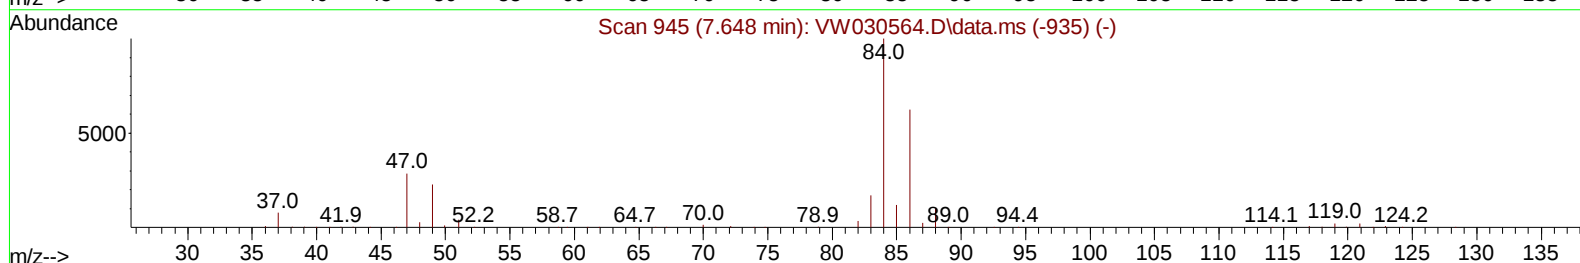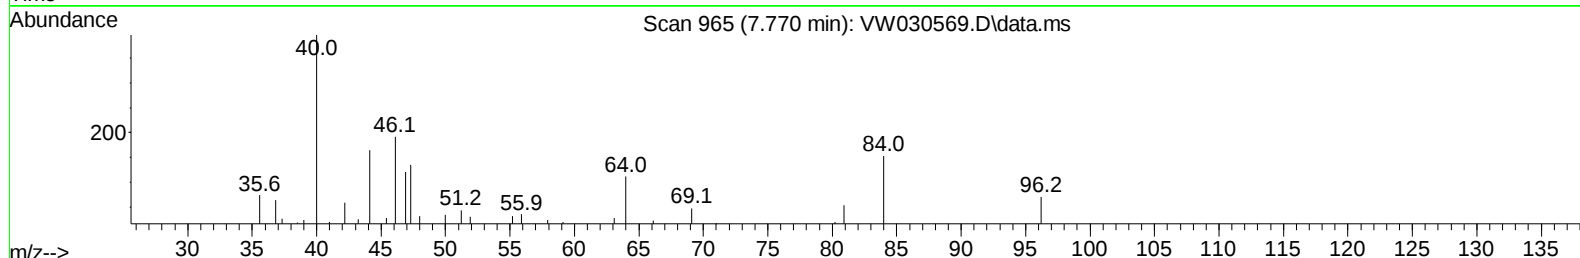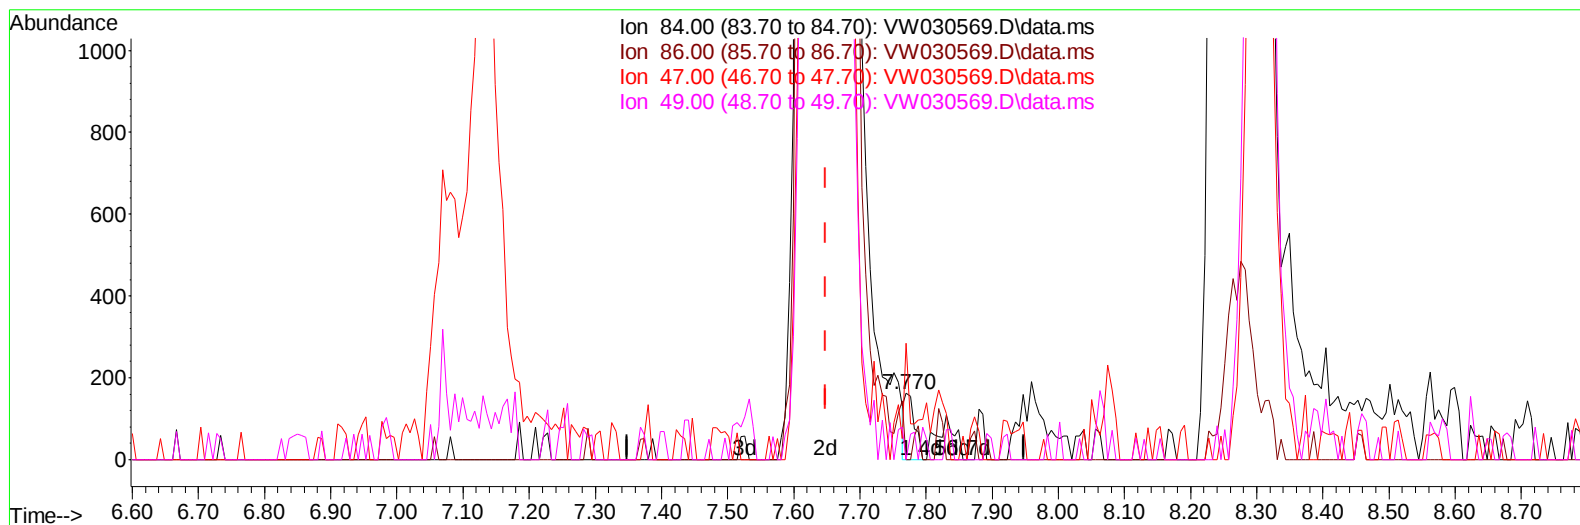

TIC: VW030569.D\data.ms

(24) Chloroform-d (S)

7.770min (+ 0.122) 0.01 ug/L

response 168

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	55.95
47.00	48.90	58.33
49.00	28.60	33.33




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030569.D
Acq On : 12 Oct 2024 00:25
Operator : SY/MD
Sample : P4361-07
Misc : 3.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAY9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 14 04:49:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

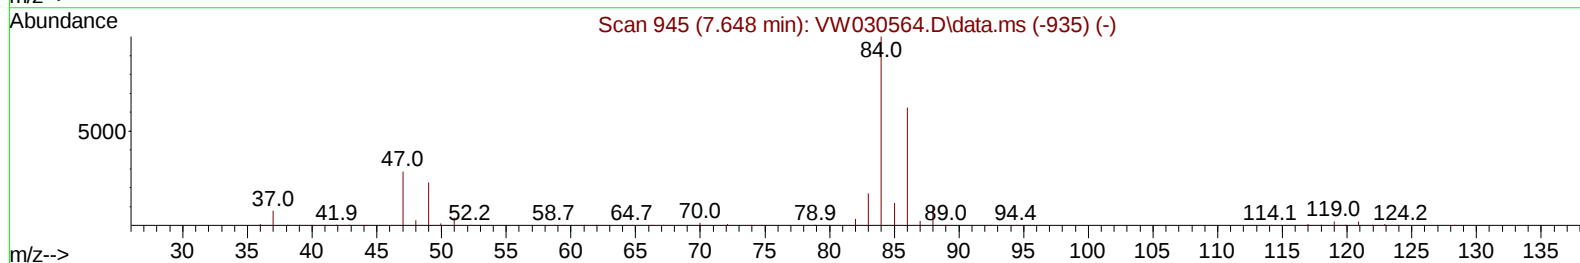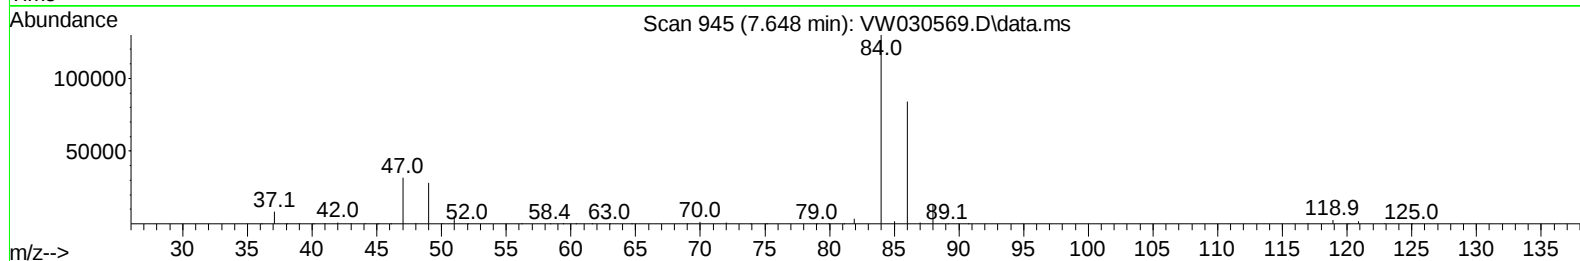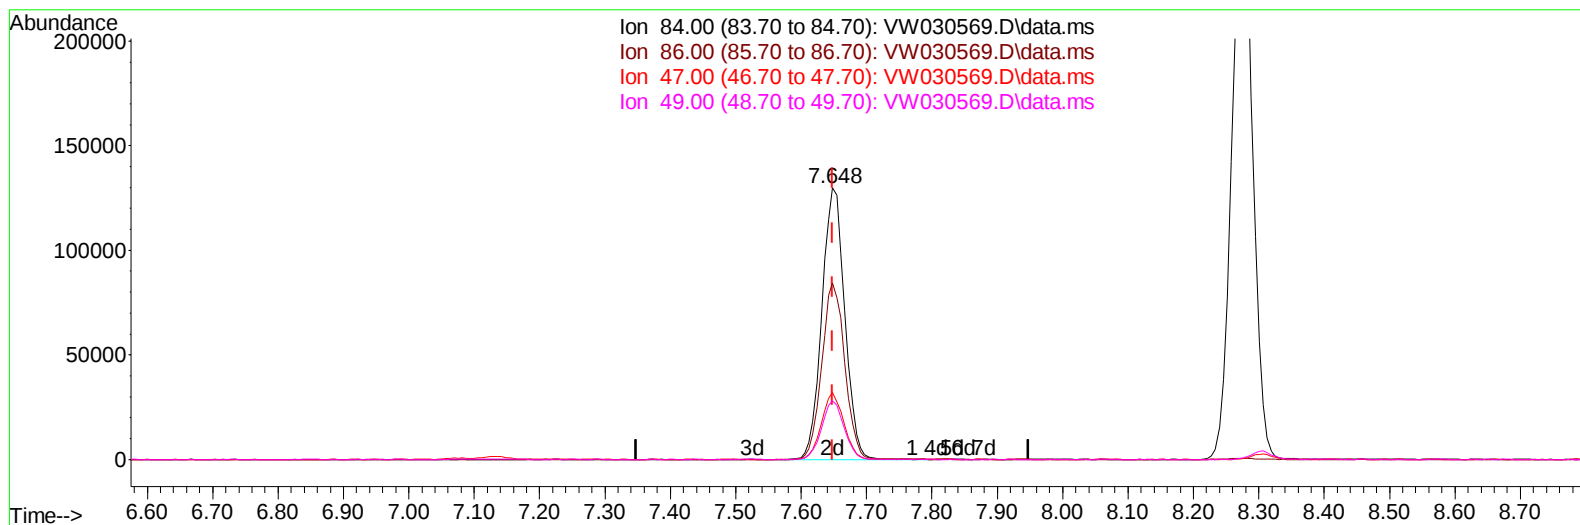

TIC: VW030569.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 23.87 ug/L m

response 315591

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.03#
47.00	48.90	0.03#
49.00	28.60	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101124\
 Data File : VW030569.D
 Acq On : 12 Oct 2024 00:25
 Operator : SY/MD
 Sample : P4361-07
 Misc : 3.35g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAY9

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:49:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	462219	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	348569	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	131123	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	181713	25.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	100.040%	
7) Chloroethane-d5	2.899	69	146247	26.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	106.360%	
11) 1,1-Dichloroethene-d2	4.021	65	72811	24.095	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	96.360%	
21) 2-Butanone-d5	7.075	46	70046	53.573	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.140%	
24) Chloroform-d	7.648	84	315591m	23.875	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.480%	
26) 1,2-Dichloroethane-d4	8.307	65	179282	26.083	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	104.320%	
32) Benzene-d6	8.276	84	601482	29.731	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	118.920%	
36) 1,2-Dichloropropane-d6	9.270	67	180497	30.397	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	121.600%#	
41) Toluene-d8	10.325	98	475925	25.770	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	103.080%	
43) trans-1,3-Dichloroprop...	10.575	79	66568	26.773	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	107.080%	
47) 2-Hexanone-d5	10.922	63	55517	72.590	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	145.180%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	126194	28.938	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	115.760%	
66) 1,2-Dichlorobenzene-d4	13.848	152	110686	24.948	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.800%	
Target Compounds						
13) Acetone	4.125	43	12095	6.319	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030569.D
Acq On : 12 Oct 2024 00:25
Operator : SY/MD
Sample : P4361-07
Misc : 3.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAY9

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:49:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

