




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030572.D
Acq On : 12 Oct 2024 01:37
Operator : SY/MD
Sample : P4361-12
Misc : 5.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAZ3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 14 04:50:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

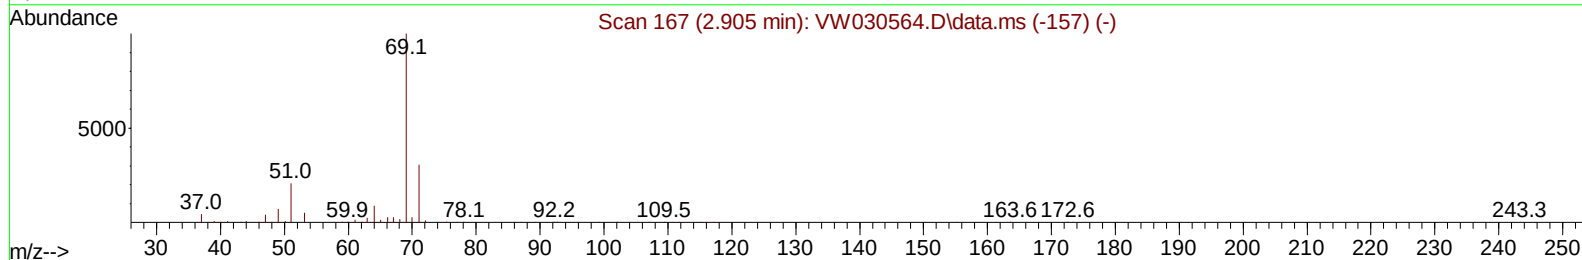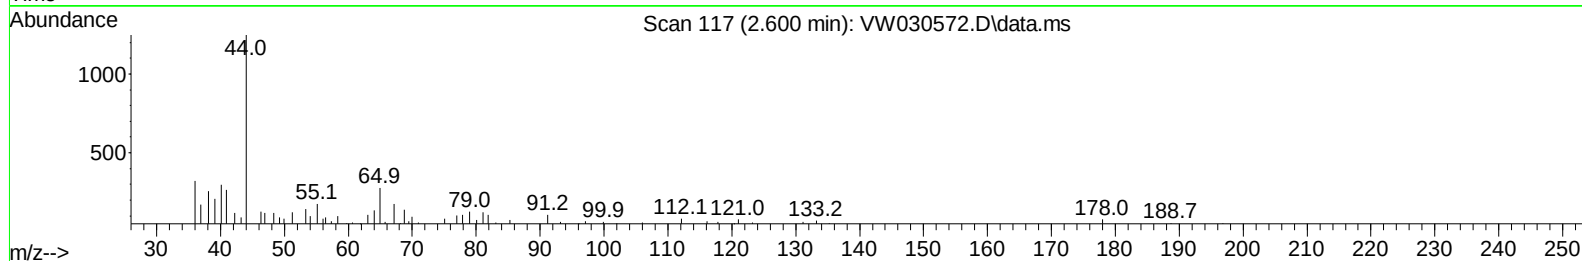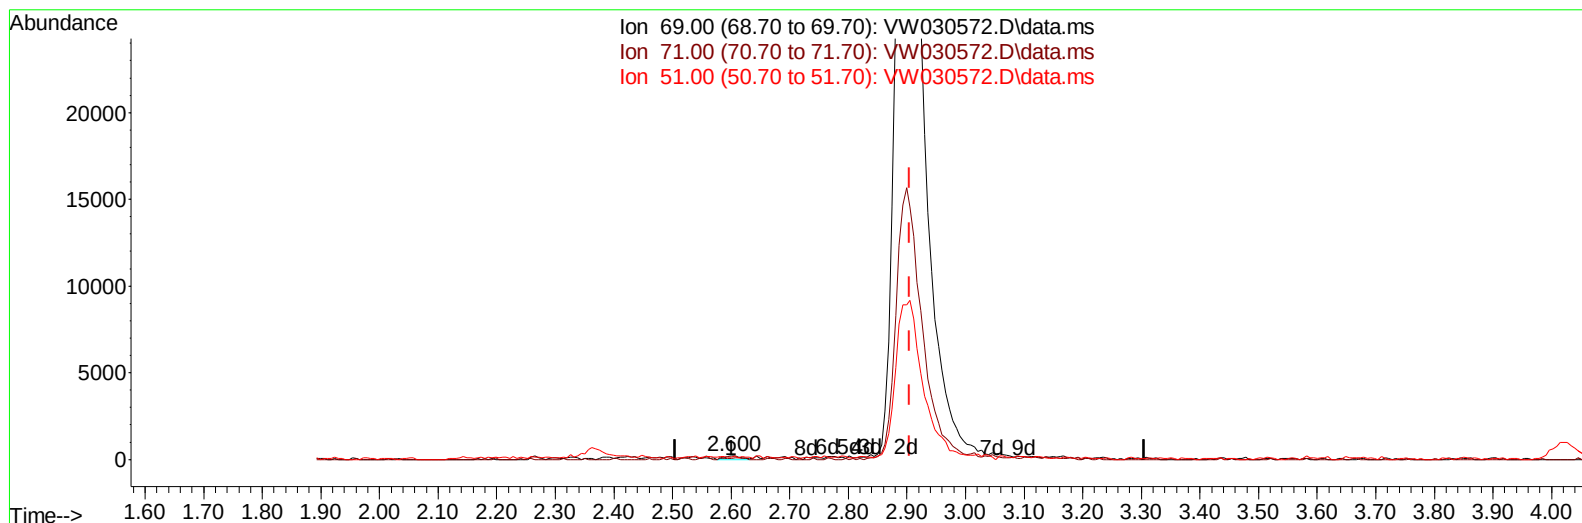

TIC: VW030572.D\data.ms

(7) Chloroethane-d5 (S)

2.600min (-0.305) 0.08 ug/L

response 395

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	23.80
51.00	10.20	7.34
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030572.D
 Acq On : 12 Oct 2024 01:37
 Operator : SY/MD
 Sample : P4361-12
 Misc : 5.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ3

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:50:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

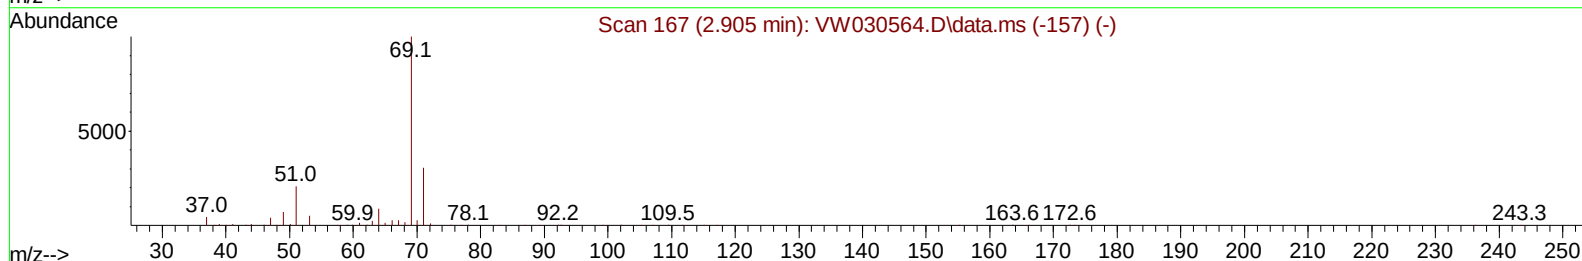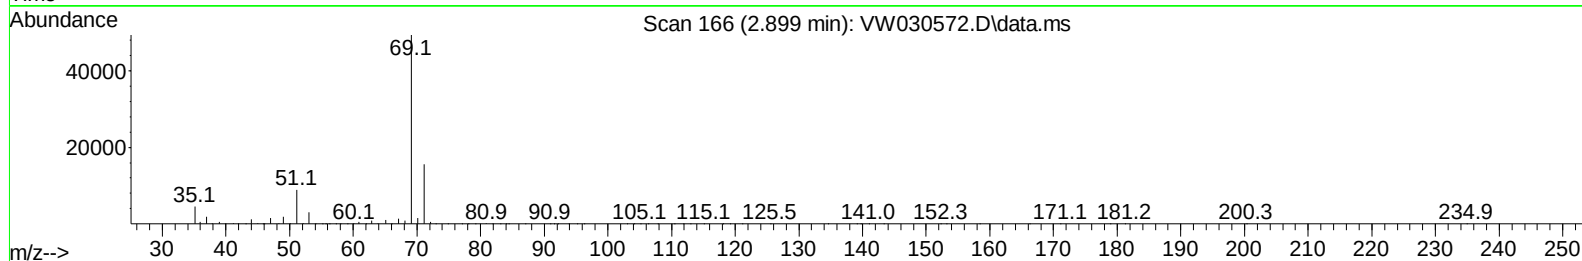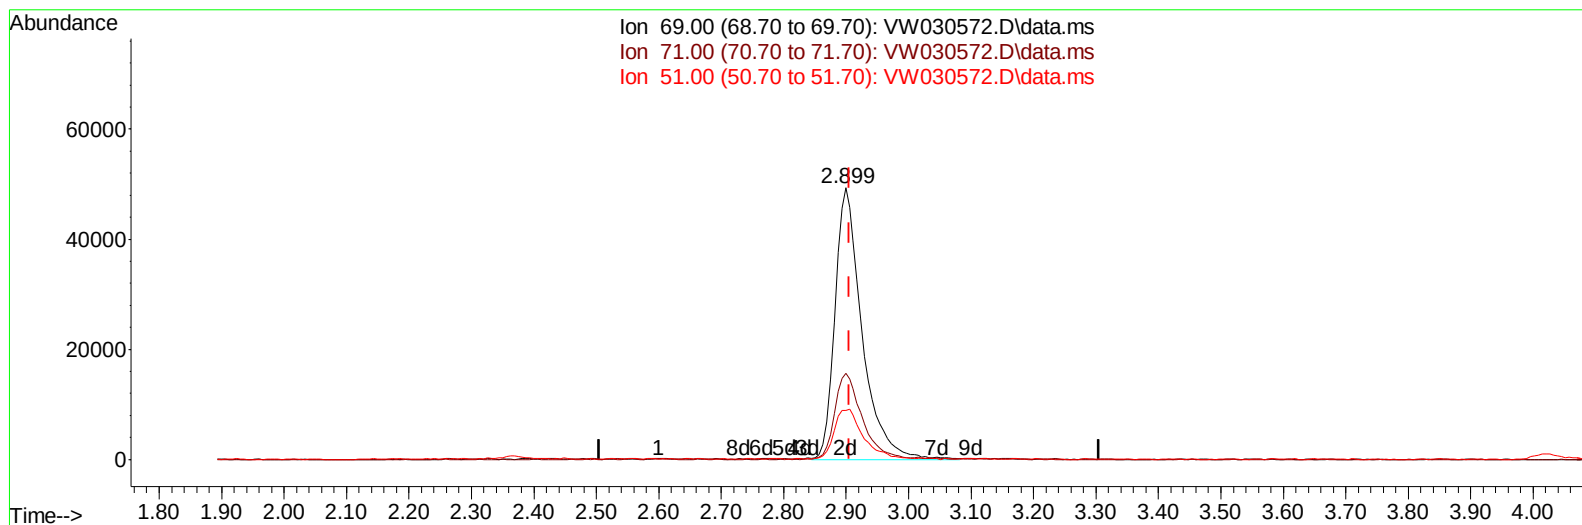

TIC: VW030572.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.006) 29.90 ug/L m

response 149608

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	0.06#
51.00	10.20	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101124\
 Data File : VW030572.D
 Acq On : 12 Oct 2024 01:37
 Operator : SY/MD
 Sample : P4361-12
 Misc : 5.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ3

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:50:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		420533	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		295349	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		95021	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		178971	27.075	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	108.320%	
7) Chloroethane-d5	2.899	69		149608m	29.900	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	119.600%	
11) 1,1-Dichloroethene-d2	4.021	65		67164	24.429	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	97.720%	
21) 2-Butanone-d5	7.081	46		58676	49.325	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	98.660%	
24) Chloroform-d	7.654	84		290238	24.133	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	96.520%	
26) 1,2-Dichloroethane-d4	8.307	65		167074	26.716	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	106.880%	
32) Benzene-d6	8.276	84		538662	31.423	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	125.680%	
36) 1,2-Dichloropropane-d6	9.270	67		168419	33.474	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	133.880%#	
41) Toluene-d8	10.325	98		408147	26.082	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	104.320%	
43) trans-1,3-Dichloroprop...	10.581	79		56855	26.986	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	107.960%	
47) 2-Hexanone-d5	10.922	63		46359	71.538	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	143.080%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		114430	30.969	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	123.880%#	
66) 1,2-Dichlorobenzene-d4	13.854	152		85511	26.597	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	106.400%	
Target Compounds							
13) Acetone	4.143	43		8730	5.013	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030572.D
Acq On : 12 Oct 2024 01:37
Operator : SY/MD
Sample : P4361-12
Misc : 5.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAZ3

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:50:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

