

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030570.D
 Acq On : 12 Oct 2024 00:49
 Operator : SY/MD
 Sample : P4361-08
 Misc : 3.53g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ0

Quant Time: Oct 14 04:50:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	462393	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	336444	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114321	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	166287	22.879	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.520%
7) Chloroethane-d5	2.899	69	139154	25.293	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.160%
11) 1,1-Dichloroethene-d2	4.021	65	66180	21.892	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.560%
21) 2-Butanone-d5	7.081	46	52215	39.920	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.840%
24) Chloroform-d	7.648	84	281993	21.325	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.320%
26) 1,2-Dichloroethane-d4	8.307	65	154569	22.479	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.920%
32) Benzene-d6	8.276	84	539332	27.620	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.480%
36) 1,2-Dichloropropane-d6	9.270	67	160341	27.976	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.920%
41) Toluene-d8	10.319	98	428673	24.048	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.200%
43) trans-1,3-Dichloroprop...	10.575	79	54892	22.872	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.480%
47) 2-Hexanone-d5	10.922	63	43047	58.313	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.620%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	103637	24.622	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.480%
66) 1,2-Dichlorobenzene-d4	13.849	152	86526	22.369	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.480%
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	13439	7.018	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030570.D
Acq On : 12 Oct 2024 00:49
Operator : SY/MD
Sample : P4361-08
Misc : 3.53g/10mL/MSVOA_W/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAZ0

Quant Time: Oct 14 04:50:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

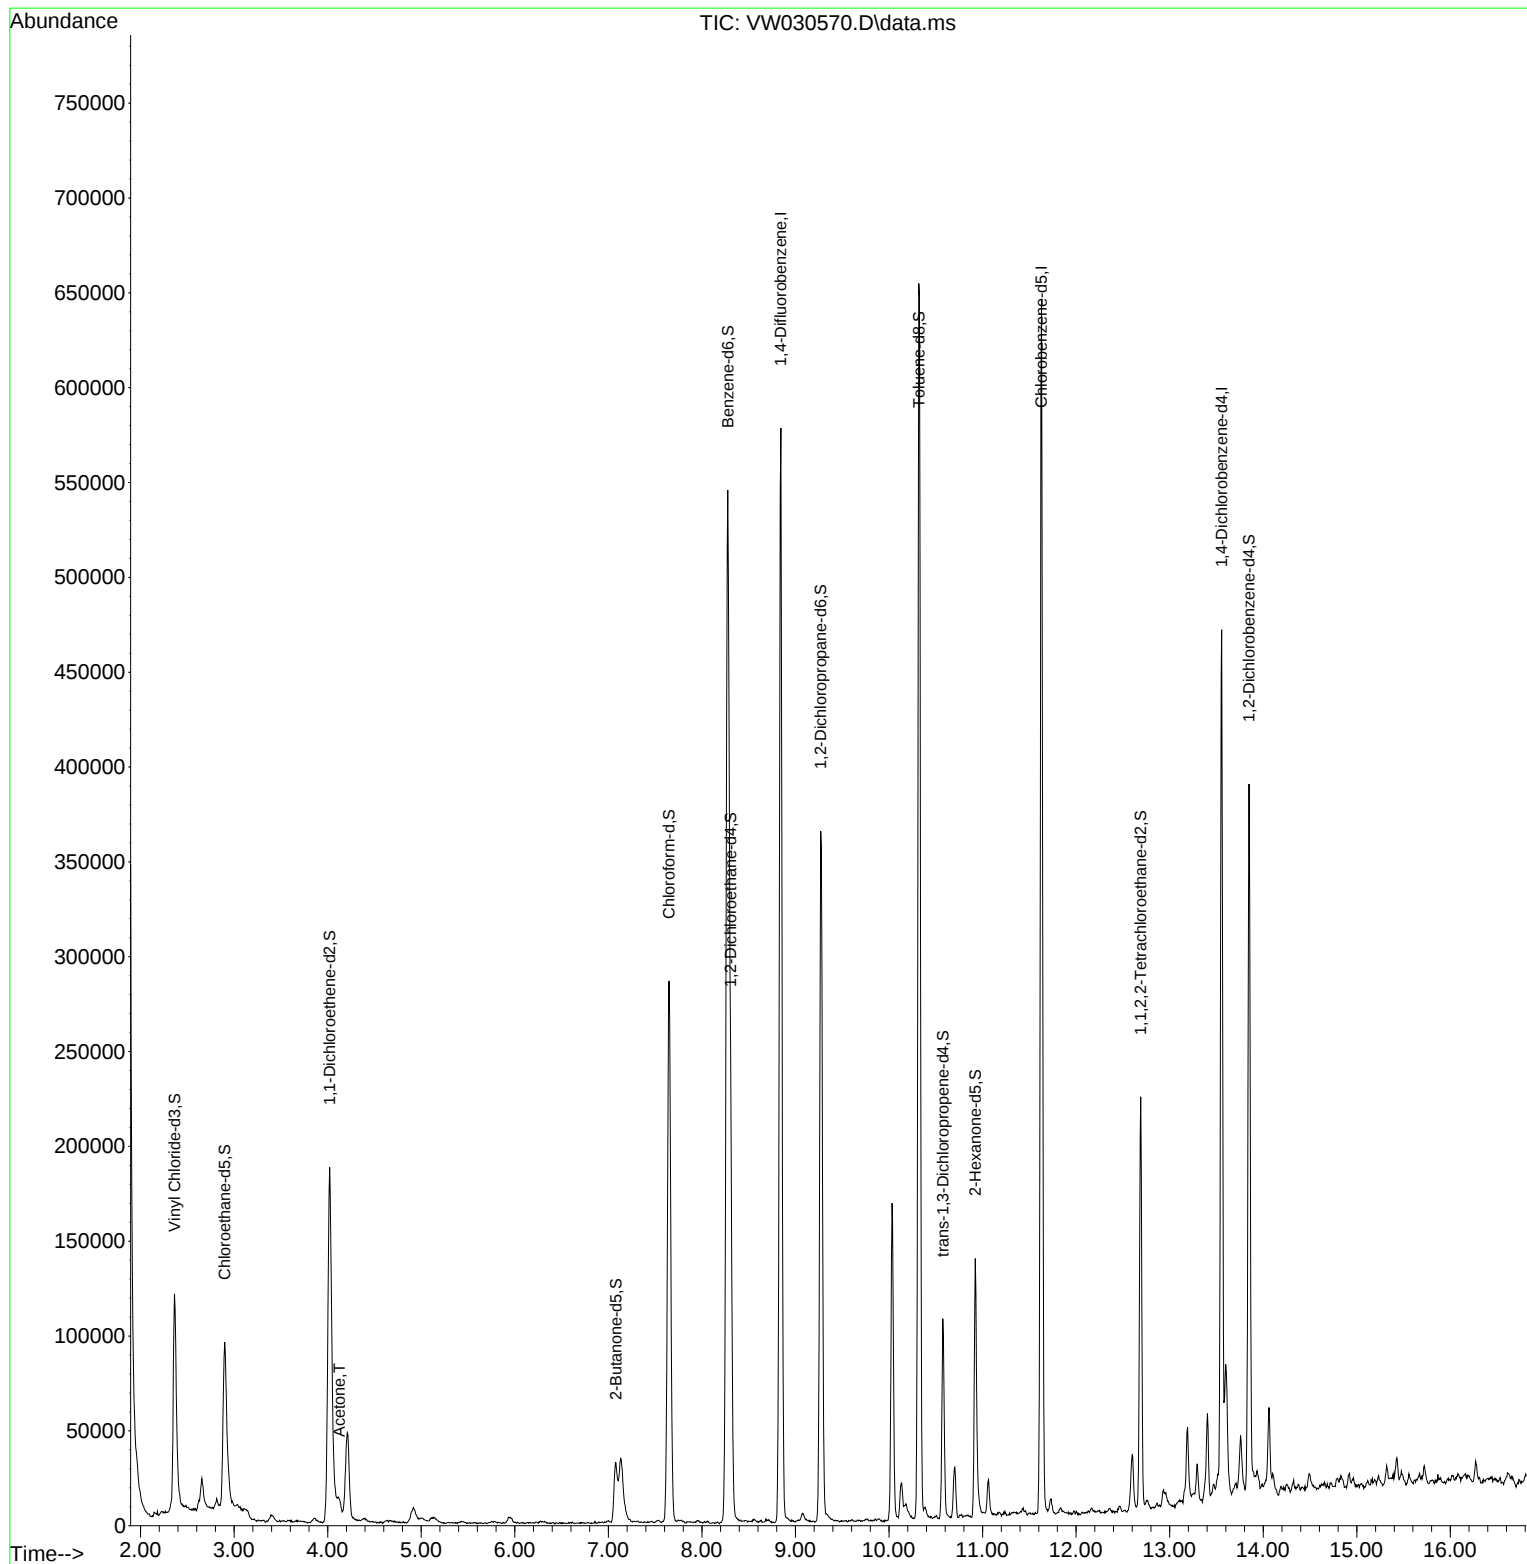

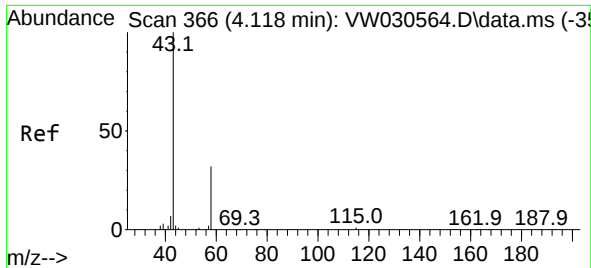

#13
 Acetone
 Concen: 7.018 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.007 min
 Lab File: VW030570.D
 Acq: 12 Oct 2024 00:49

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ0

Tgt Ion: 43 Resp: 13439
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 57.6

