

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030573.D
 Acq On : 12 Oct 2024 02:01
 Operator : SY/MD
 Sample : P4361-13
 Misc : 3.24g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ4

Quant Time: Oct 14 04:50:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	345992	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	269126	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	94638	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	132532	24.369	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.480%
7) Chloroethane-d5	2.899	69	104834	25.466	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.880%
11) 1,1-Dichloroethene-d2	4.021	65	50854	22.482	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.920%
21) 2-Butanone-d5	7.075	46	47947	48.990	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.980%
24) Chloroform-d	7.648	84	215733	21.803	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	8.307	65	128132	24.903	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.600%
32) Benzene-d6	8.270	84	413273	26.458	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.840%
36) 1,2-Dichloropropane-d6	9.270	67	126823	27.663	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.640%
41) Toluene-d8	10.319	98	328199	23.016	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.080%
43) trans-1,3-Dichloroprop...	10.575	79	43190	22.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.000%
47) 2-Hexanone-d5	10.922	63	37144	62.903	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91364	27.136	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.560%
66) 1,2-Dichlorobenzene-d4	13.848	152	76329	23.837	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.360%
Target Compounds					Qvalue	
13) Acetone	4.131	43	9237	6.447	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030573.D
Acq On : 12 Oct 2024 02:01
Operator : SY/MD
Sample : P4361-13
Misc : 3.24g/10mL/MSVOA_W/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAZ4

Quant Time: Oct 14 04:50:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

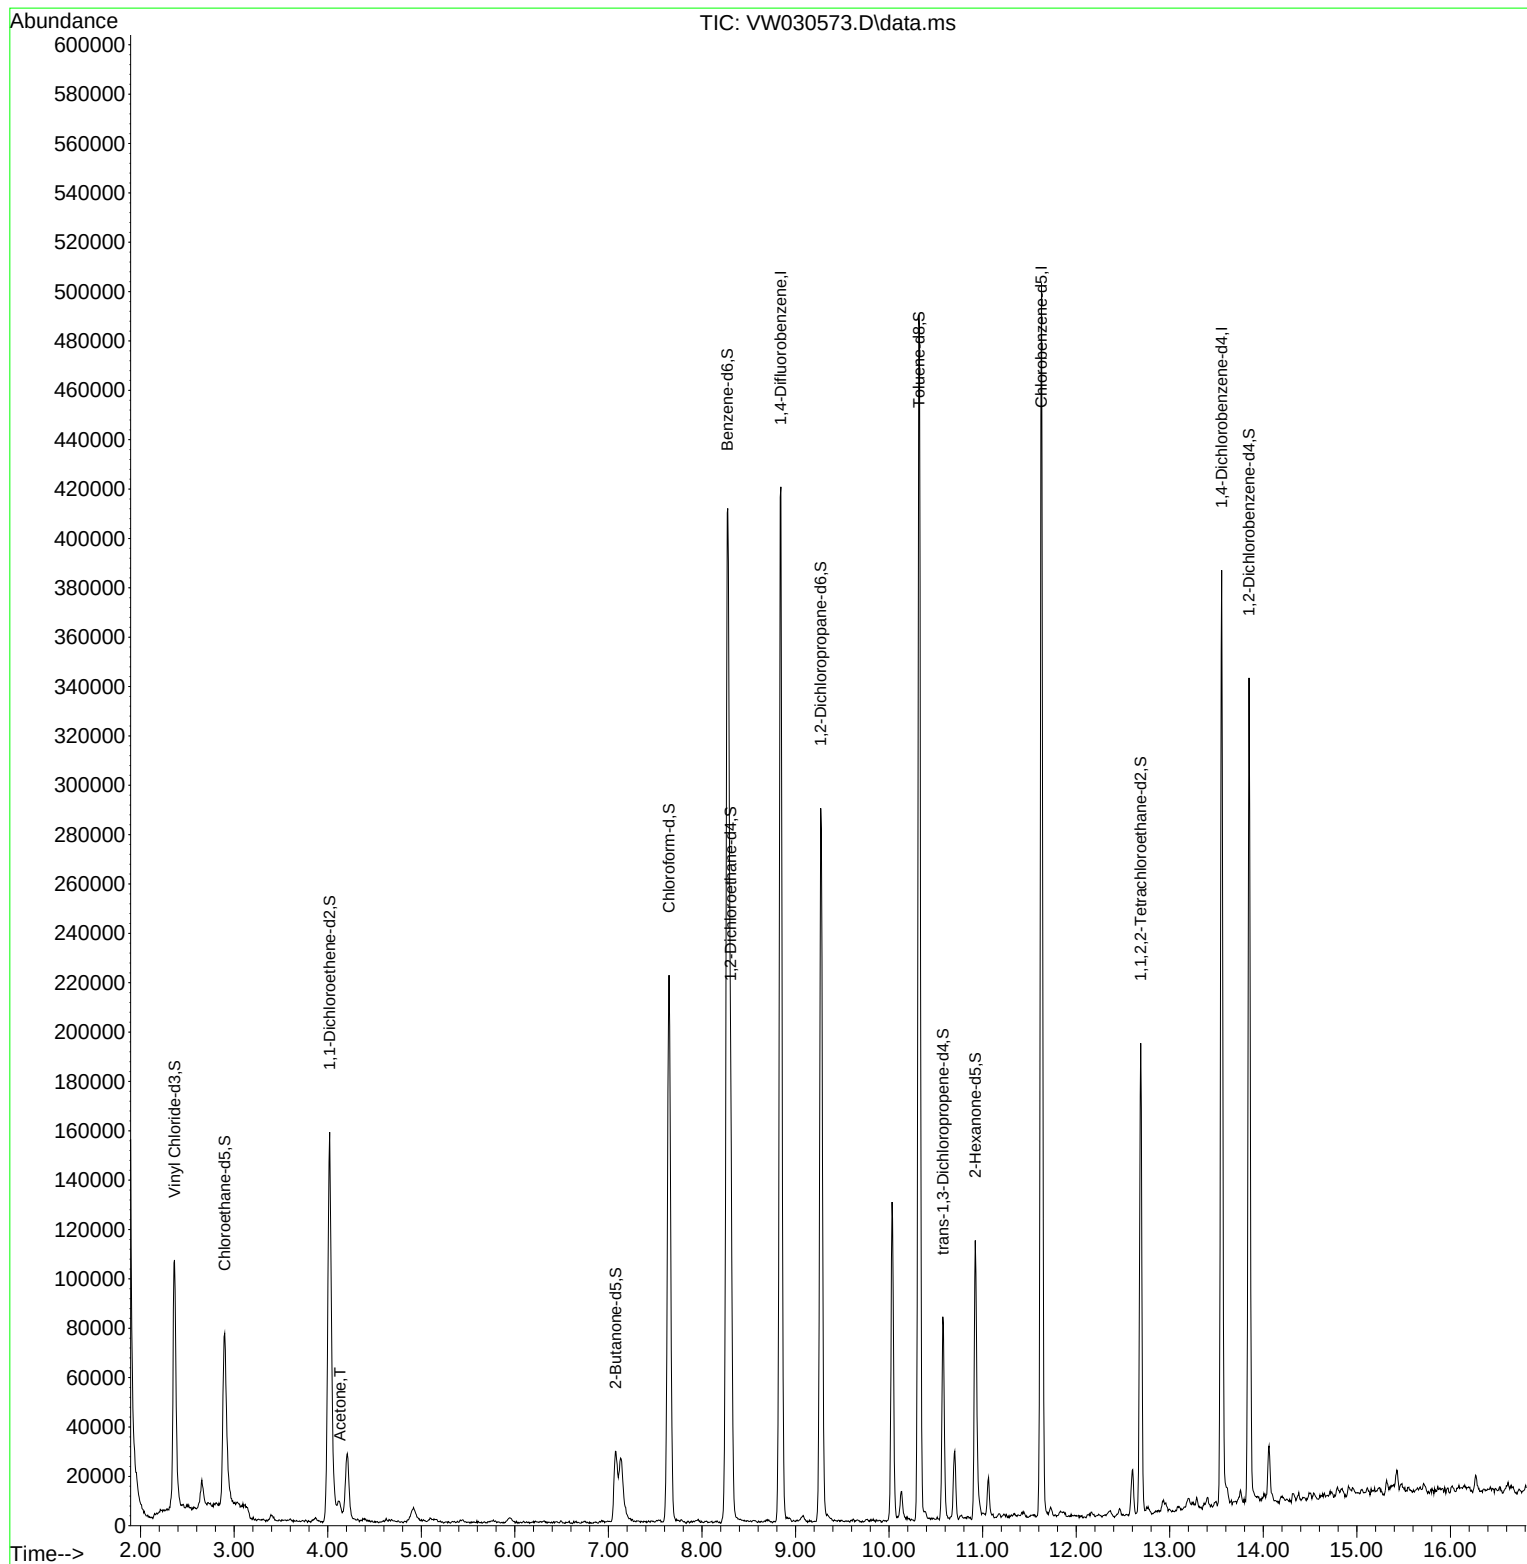

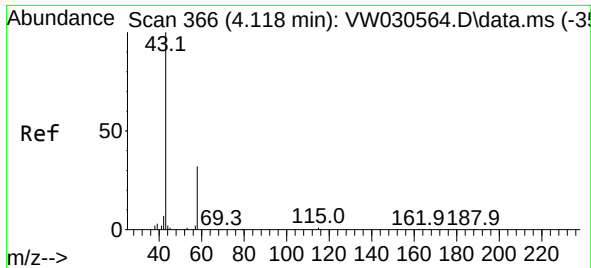

#13
 Acetone
 Concen: 6.447 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW030573.D
 Acq: 12 Oct 2024 02:01

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ4

Tgt Ion: 43 Resp: 9237
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 57.6

