

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030574.D
 Acq On : 12 Oct 2024 02:25
 Operator : SY/MD
 Sample : P4350-11
 Misc : 3.14g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK2

Quant Time: Oct 14 04:50:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	346206	25.000	ug/L	-0.01
28) Chlorobenzene-d5	11.629	117	305680	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	101766	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	100627	18.491	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.960%
7) Chloroethane-d5	2.893	69	94228	22.875	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.520%
11) 1,1-Dichloroethene-d2	4.021	65	43427	19.187	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.760%
21) 2-Butanone-d5	7.075	46	52826	53.941	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.880%
24) Chloroform-d	7.648	84	228174	23.046	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	8.307	65	149610	29.059	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	116.240%
32) Benzene-d6	8.276	84	426051	24.014	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.040%
36) 1,2-Dichloropropane-d6	9.270	67	139567	26.802	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.200%
41) Toluene-d8	10.319	98	368658	22.762	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.040%
43) trans-1,3-Dichloroprop...	10.575	79	51196	23.479	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.920%
47) 2-Hexanone-d5	10.922	63	40896	60.975	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.940%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	114500	29.940	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	83853	24.352	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.400%
Target Compounds					Qvalue	
13) Acetone	4.125	43	13775	9.608	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030574.D
Acq On : 12 Oct 2024 02:25
Operator : SY/MD
Sample : P4350-11
Misc : 3.14g/10mL/MSVOA_W/SOIL/A
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAK2

Quant Time: Oct 14 04:50:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

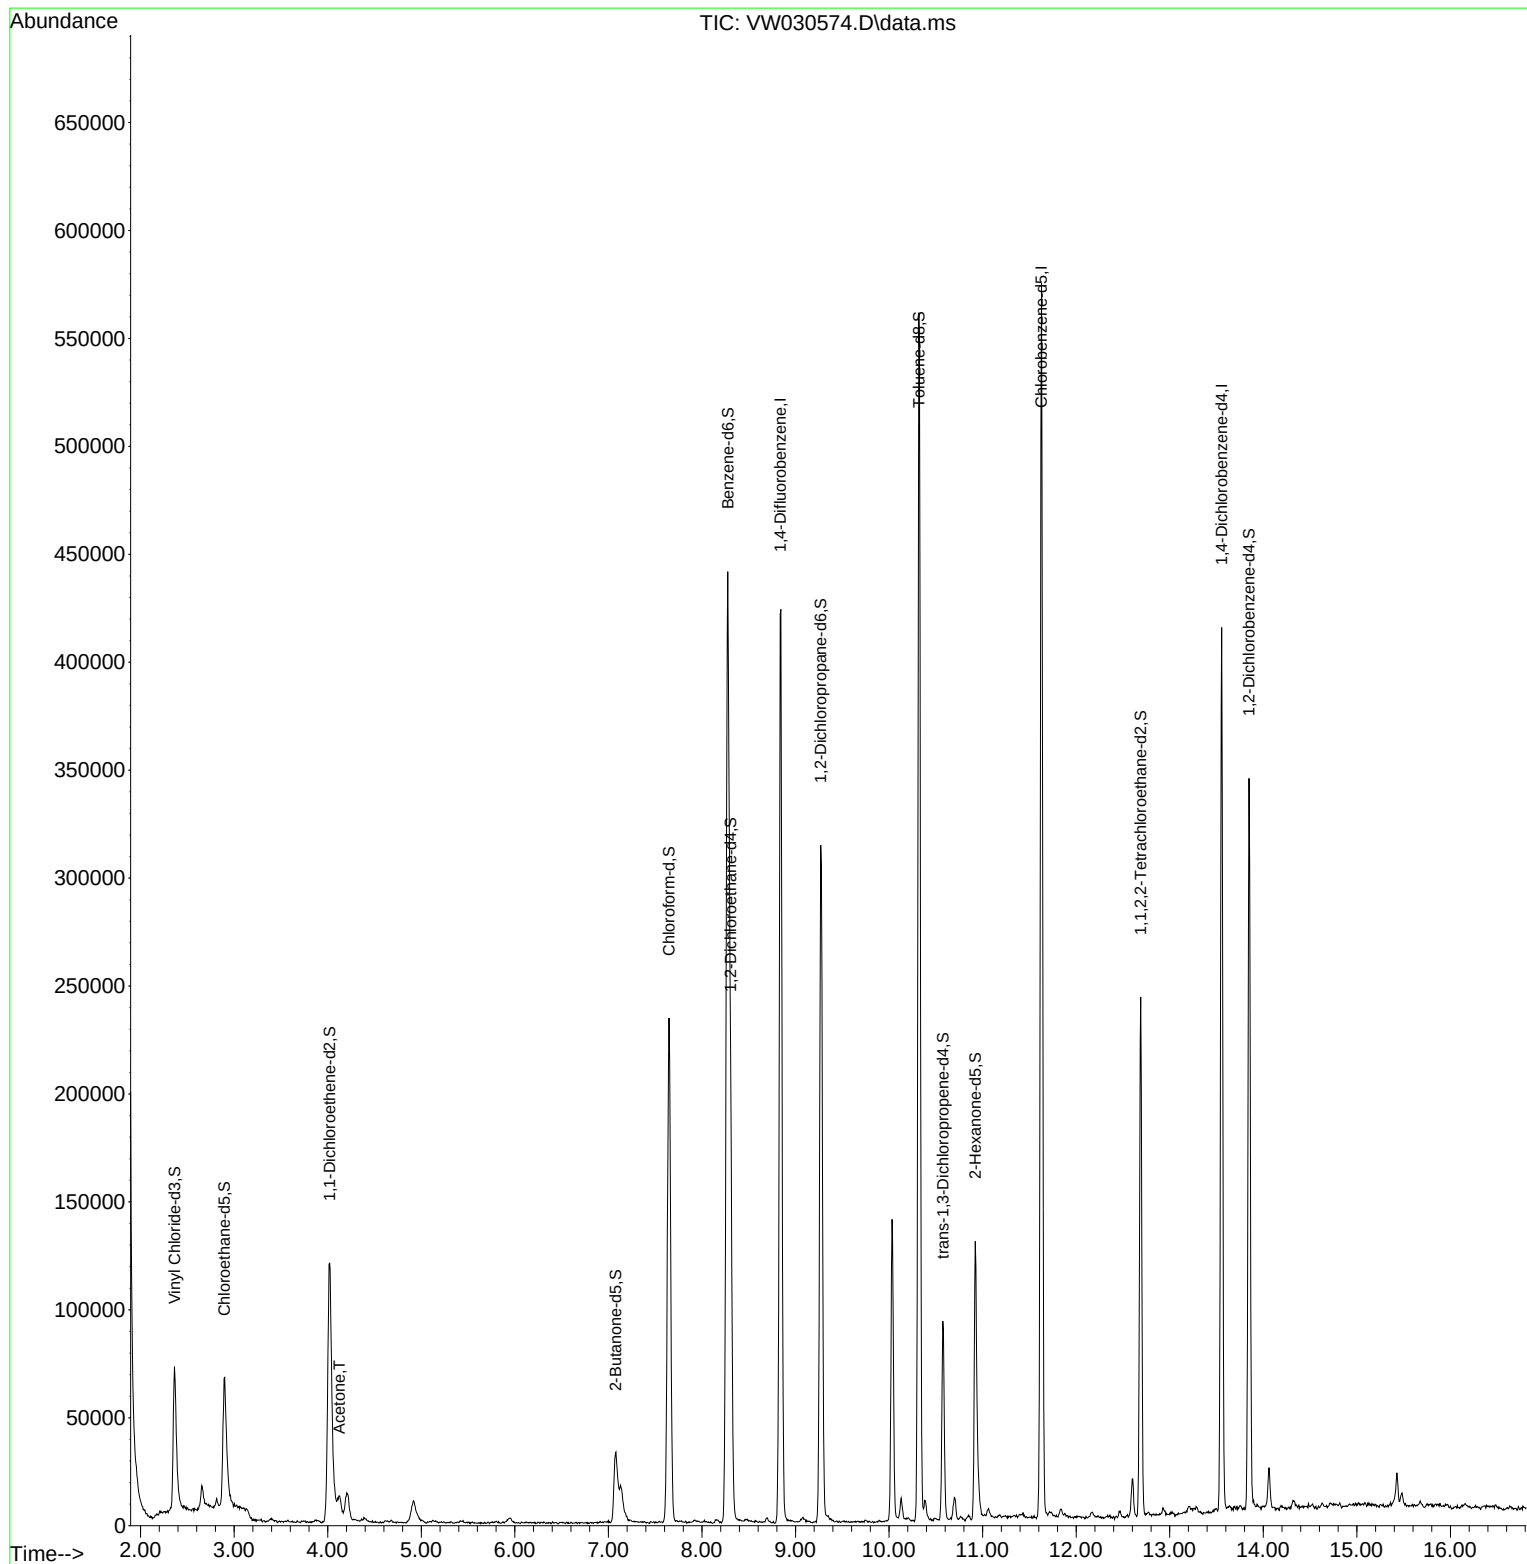

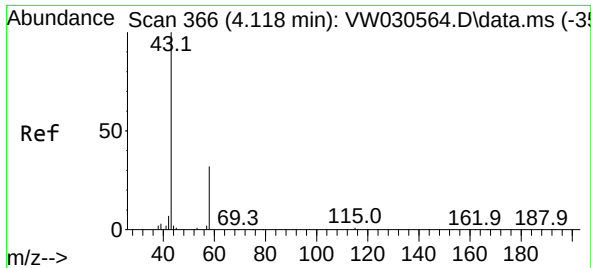

#13
 Acetone
 Concen: 9.608 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030574.D
 Acq: 12 Oct 2024 02:25

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK2

Tgt Ion: 43 Resp: 13775
 Ion Ratio Lower Upper
 43 100
 58 21.4 0.0 57.6

