

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
 Data File : VW030578.D
 Acq On : 12 Oct 2024 04:01
 Operator : SY/MD
 Sample : P4361-14
 Misc : 4.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ5

Quant Time: Oct 14 04:51:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 14 04:33:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	409089	25.000	ug/L	-0.01
28) Chlorobenzene-d5	11.629	117	316871	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	115432	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	157041	24.422	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.680%
7) Chloroethane-d5	2.899	69	133253	27.376	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.520%
11) 1,1-Dichloroethene-d2	4.021	65	59345	22.189	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	88.760%
21) 2-Butanone-d5	7.075	46	63871	55.194	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.380%
24) Chloroform-d	7.648	84	266532	22.782	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.120%
26) 1,2-Dichloroethane-d4	8.301	65	153080	25.163	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.640%
32) Benzene-d6	8.276	84	505326	27.477	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.920%
36) 1,2-Dichloropropane-d6	9.270	67	154480	28.618	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.480%
41) Toluene-d8	10.325	98	402126	23.952	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	10.575	79	55809	24.691	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.760%
47) 2-Hexanone-d5	10.922	63	51130	73.541	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.080%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	113402	28.606	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.440%
66) 1,2-Dichlorobenzene-d4	13.854	152	102040	26.126	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.520%
Target Compounds						
13) Acetone	4.124	43	12099	7.142	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101124\
Data File : VW030578.D
Acq On : 12 Oct 2024 04:01
Operator : SY/MD
Sample : P4361-14
Misc : 4.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAZ5

Quant Time: Oct 14 04:51:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 14 04:33:53 2024
Response via : Initial Calibration

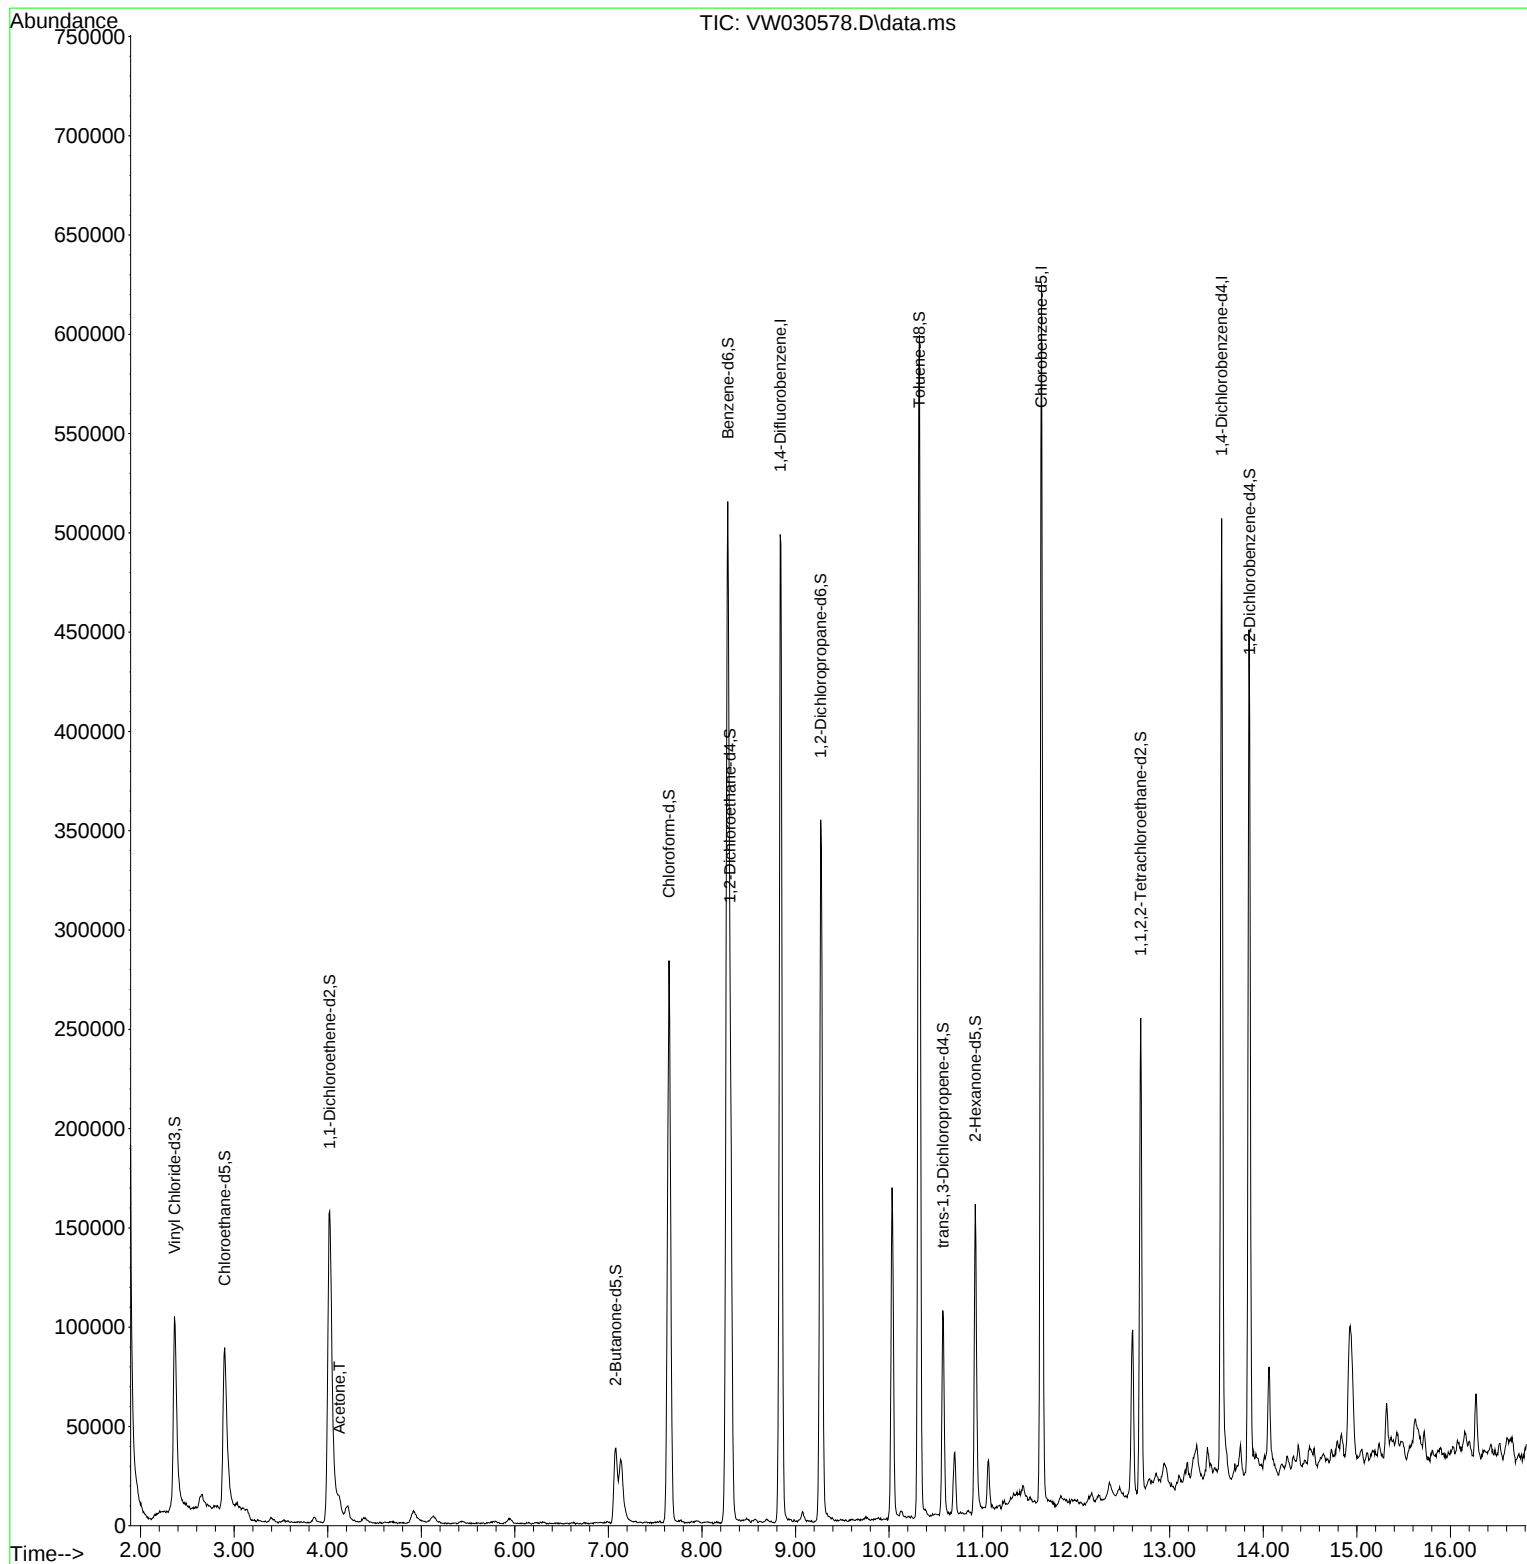

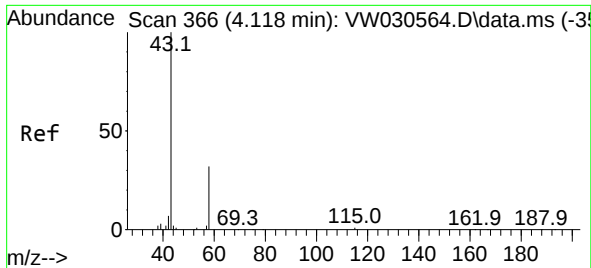

#13
 Acetone
 Concen: 7.142 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030578.D
 Acq: 12 Oct 2024 04:01

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAZ5

Tgt Ion: 43 Resp: 12099
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 57.6

