

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101322\
 Data File : VW024897.D
 Acq On : 13 Oct 2022 11:46
 Operator : SY/VA
 Sample : VW1013SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK426

Quant Time: Oct 14 02:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 14 02:07:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	489379	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	449916	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	207669	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	121199	20.992	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.960%
7) Chloroethane-d5	2.892	69	69755	20.635	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.560%
11) 1,1-Dichloroethene-d2	4.019	63	201333	16.038	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.160%
21) 2-Butanone-d5	7.080	46	77584	42.411	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.820%
24) Chloroform-d	7.647	84	288027	20.867	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.480%
26) 1,2-Dichloroethane-d4	8.305	65	153505	21.249	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.000%
32) Benzene-d6	8.275	84	615241	21.807	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.240%
36) 1,2-Dichloropropane-d6	9.275	67	186502	21.553	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.200%
41) Toluene-d8	10.323	98	549582	21.703	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.800%
43) trans-1,3-Dichloroprop...	10.579	79	68199	20.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.120%
47) 2-Hexanone-d5	10.927	63	59004	40.670	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.340%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	134844	19.982	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.920%
66) 1,2-Dichlorobenzene-d4	13.847	152	164577	21.686	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5185	0.470	ug/L	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101322\
Data File : VW024897.D
Acq On : 13 Oct 2022 11:46
Operator : SY/VA
Sample : VW1013SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK426

Quant Time: Oct 14 02:11:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 14 02:07:33 2022
Response via : Initial Calibration

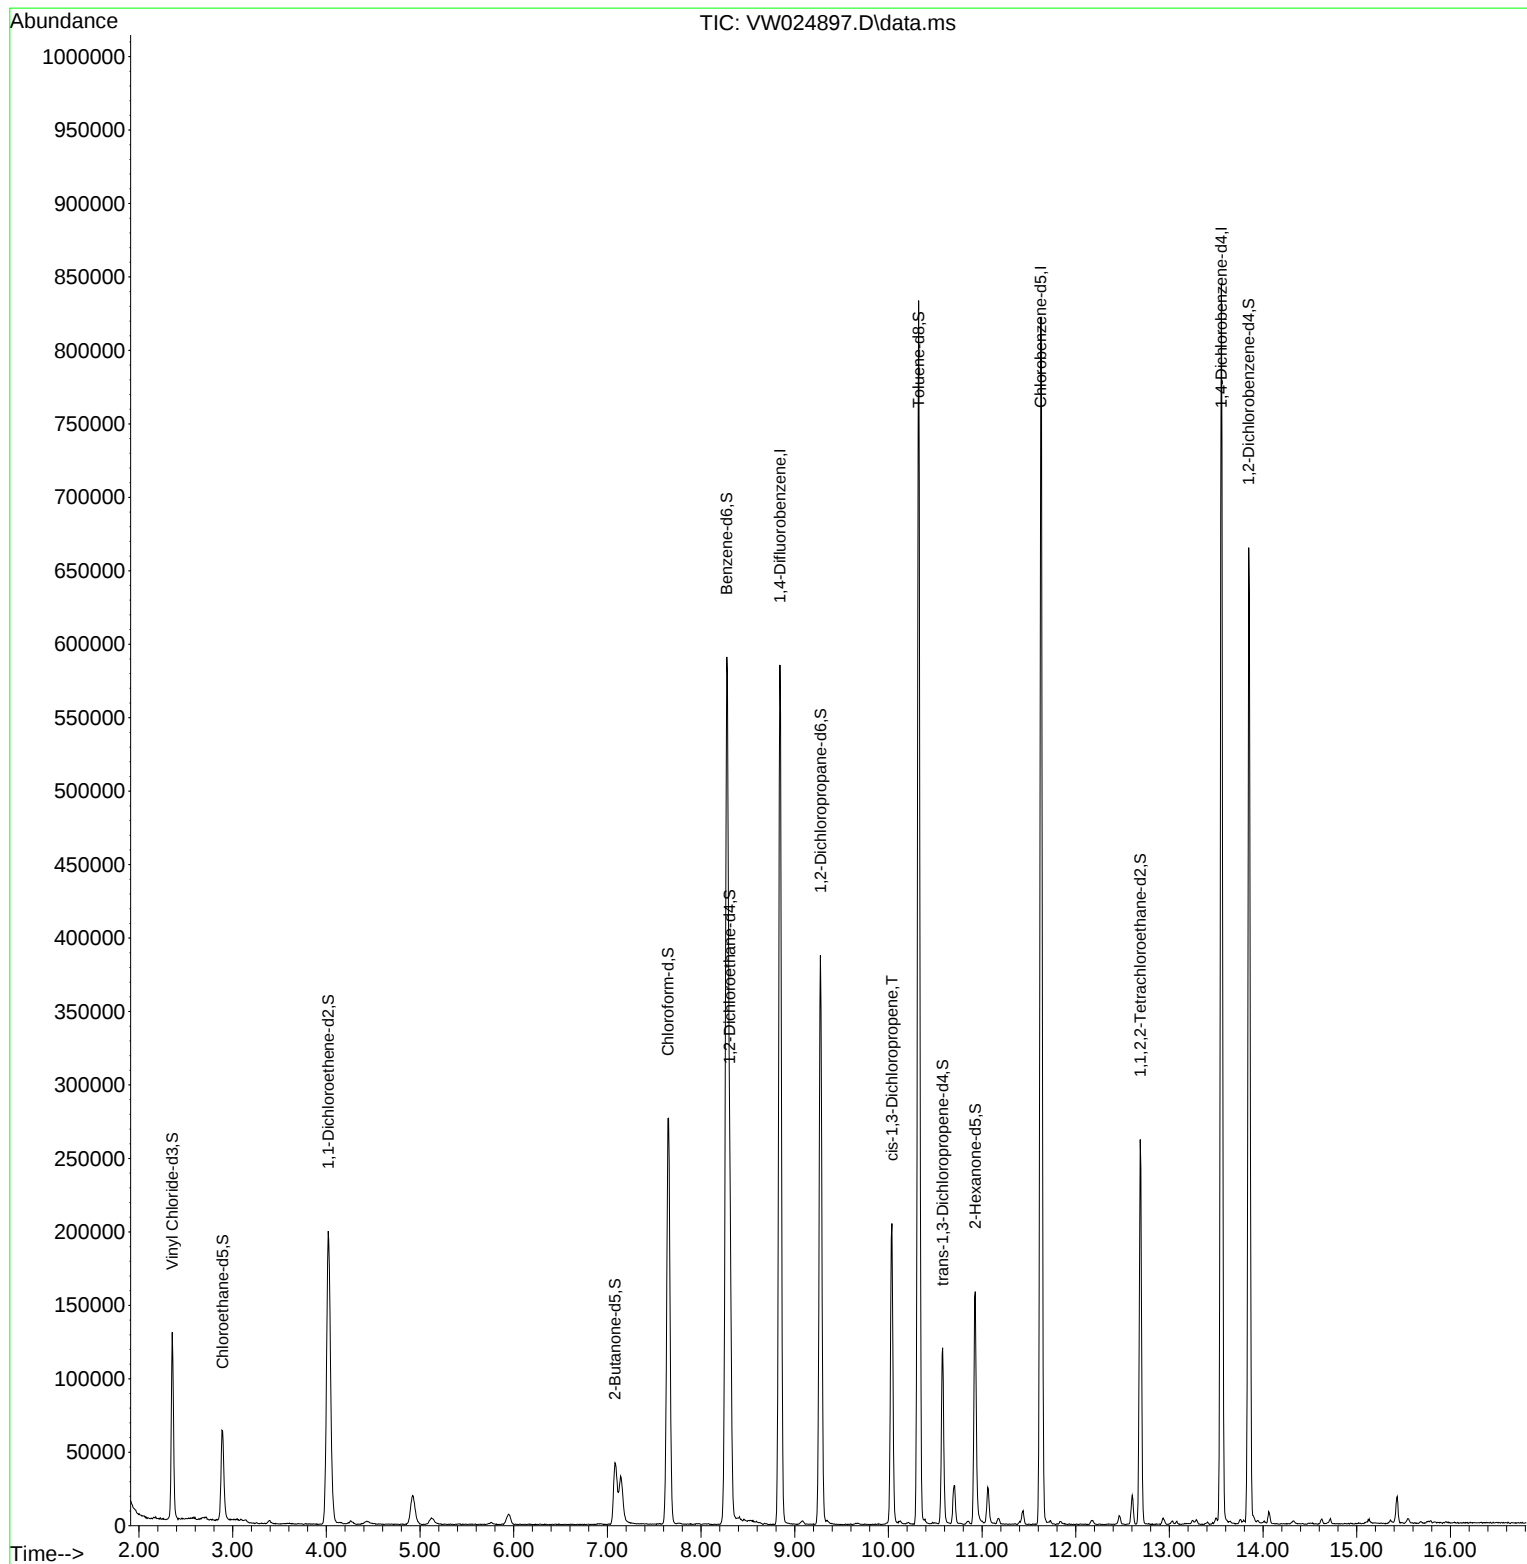

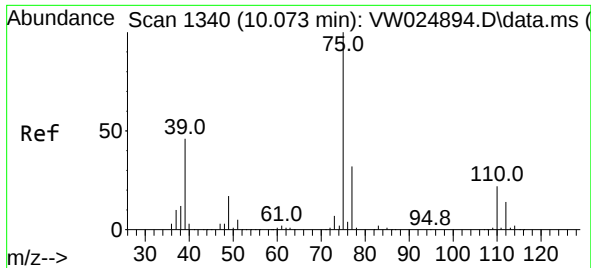

#39

cis-1,3-Dichloropropene

Concen: 0.470 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.036 min

Lab File: VW024897.D


Acq: 13 Oct 2022 11:46

Instrument :

MSVOA_W

ClientSampleId :

VBLK426

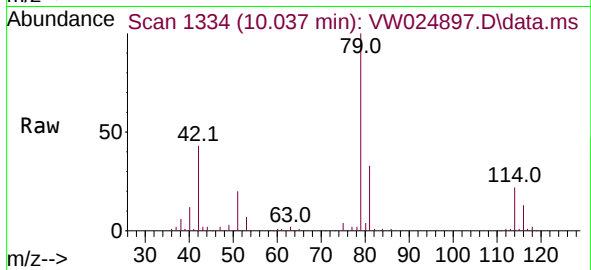

Tgt Ion: 75 Resp: 5185

Ion Ratio Lower Upper

75 100

77 62.2 21.9 40.7#

