

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101322\
 Data File : VW024908.D
 Acq On : 13 Oct 2022 16:58
 Operator : SY/VA
 Sample : N5119-03
 Misc : 4.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BC4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/14/2022
 Supervised By :Mahesh Dadoda 10/17/2022

Quant Time: Oct 14 02:14:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 14 02:07:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	474620	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	383648	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	146116	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	100471	17.943	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	71.760%	
7) Chloroethane-d5	2.885	69	65439	19.961	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	79.840%	
11) 1,1-Dichloroethene-d2	4.019	63	167609	13.767	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	55.080%	
21) 2-Butanone-d5	7.080	46	102778	57.930	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	115.860%	
24) Chloroform-d	7.653	84	304690	22.760	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	91.040%	
26) 1,2-Dichloroethane-d4	8.305	65	173236m	24.726	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	98.920%	
32) Benzene-d6	8.275	84	574033	23.861	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	95.440%	
36) 1,2-Dichloropropane-d6	9.275	67	196080	26.573	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	106.280%	
41) Toluene-d8	10.323	98	464055	21.491	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	85.960%	
43) trans-1,3-Dichloroprop...	10.579	79	62074	22.181	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	88.720%	
47) 2-Hexanone-d5	10.927	63	77971	63.027	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	126.060%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	175904	30.568	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	122.280%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	124036	23.229	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	92.920%	
Target Compounds					Qvalue	
13) Acetone	4.141	43	5112	4.118	ug/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101322\
Data File : VW024908.D
Acq On : 13 Oct 2022 16:58
Operator : SY/VA
Sample : N5119-03
Misc : 4.64g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0BC4

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 10/14/2022
Supervised By : Mahesh Dadoda 10/17/2022


Quant Time: Oct 14 02:14:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 14 02:07:33 2022
Response via : Initial Calibration

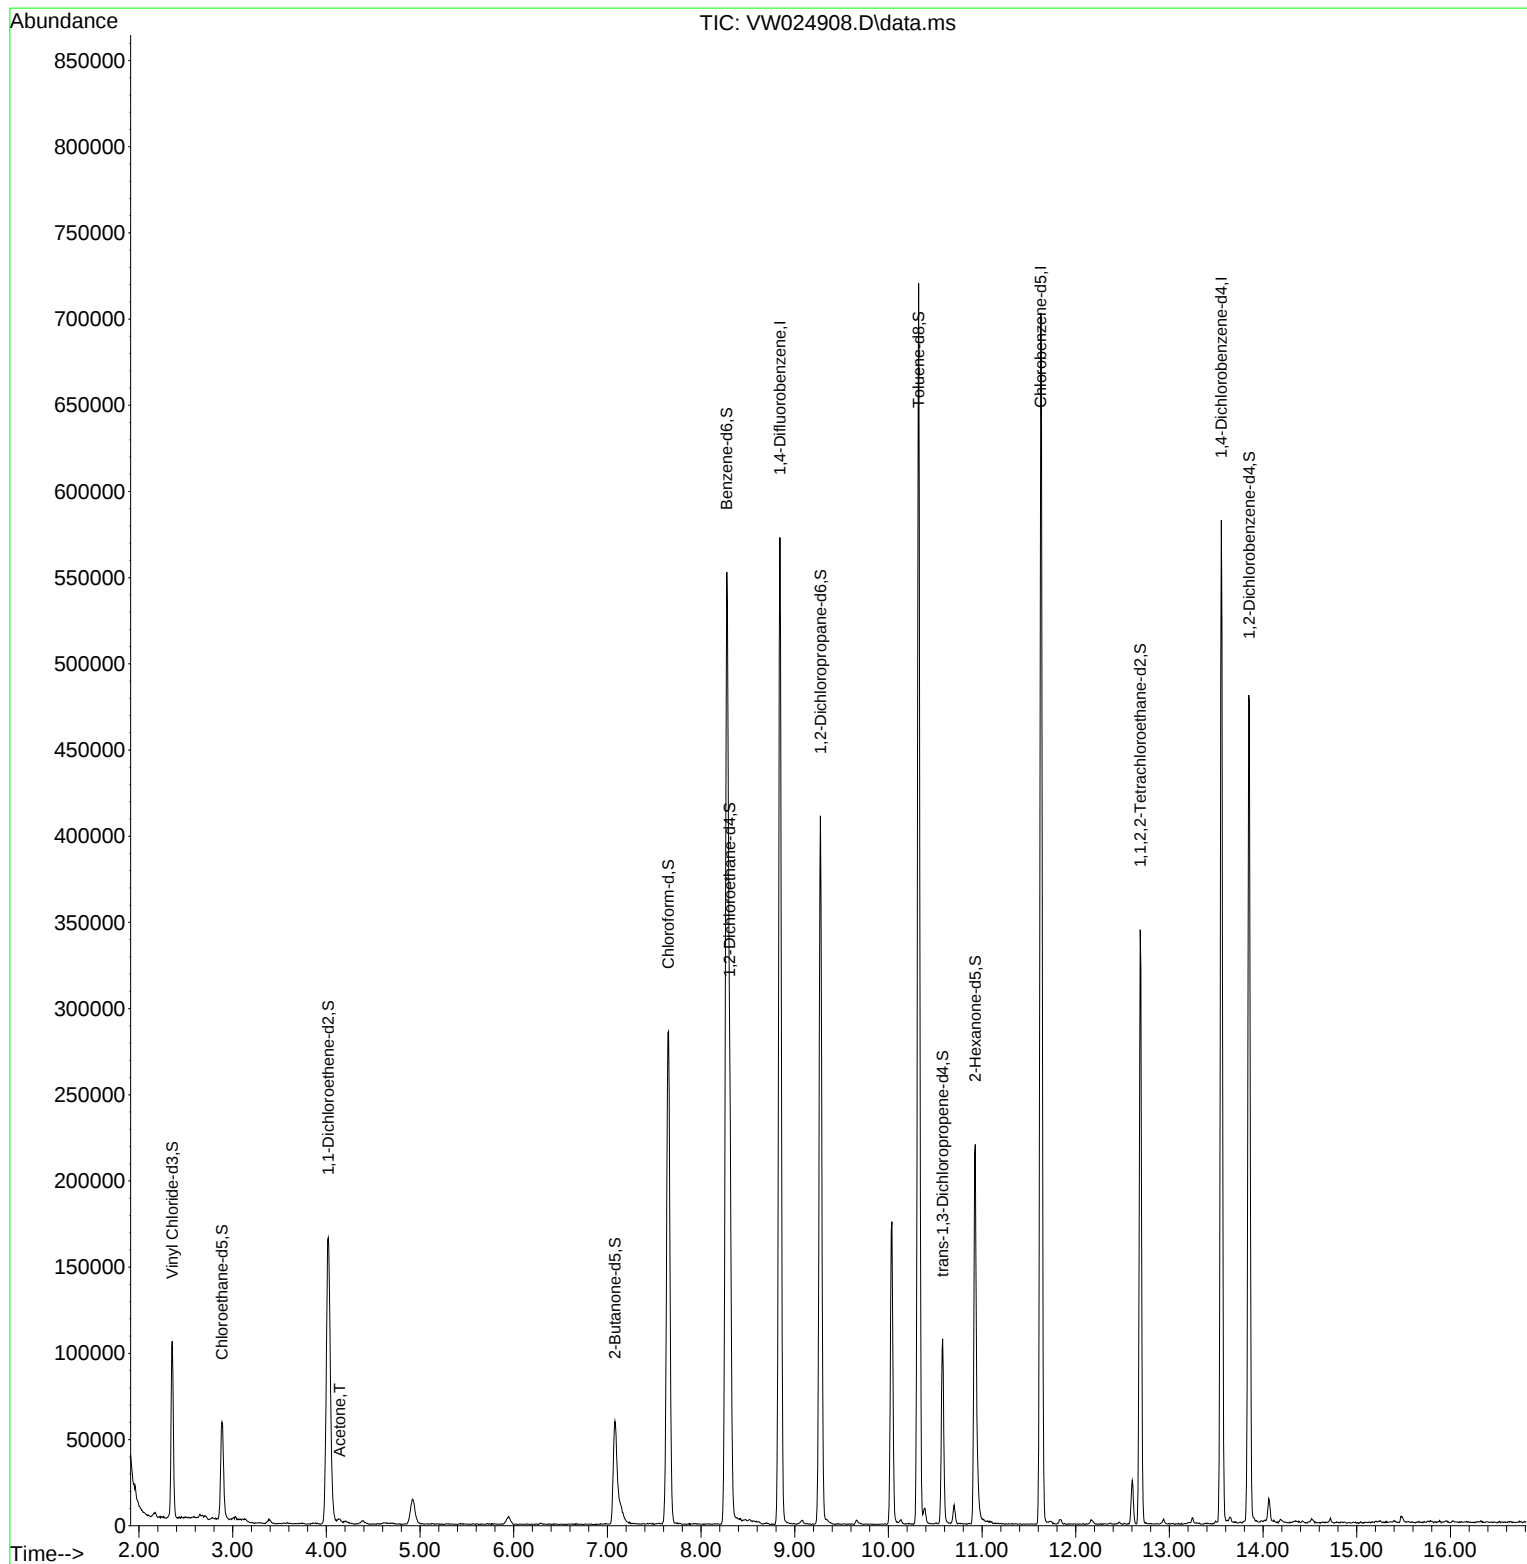

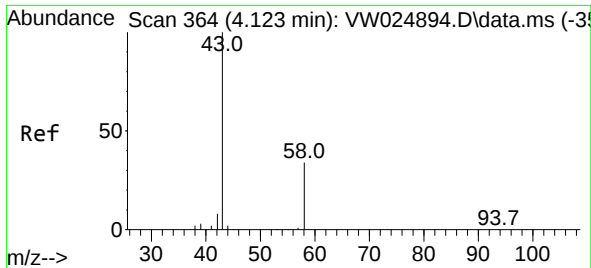

#13
 Acetone
 Concen: 4.118 ug/L
 RT: 4.141 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW024908.D
 Acq: 13 Oct 2022 16:58

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BC4

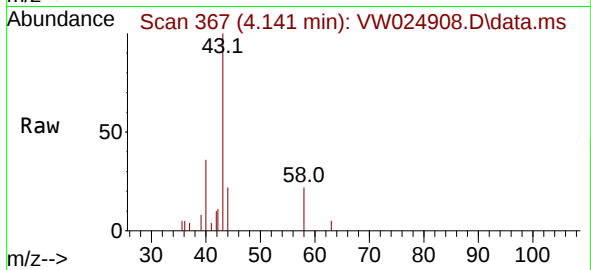

Tgt Ion: 43 Resp: 511
 Ion Ratio Lower Upper
 43 100
 58 18.9 0.0 64.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/14/2022
 Supervised By :Mahesh Dadoda 10/17/2022

