

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
 Data File : VW024916.D
 Acq On : 14 Oct 2022 09:01
 Operator : SY/VA
 Sample : VW1014SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 15 00:15:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 15 00:14:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	445400	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	405161	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	183935	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	120666	22.964	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.840%
7) Chloroethane-d5	2.885	69	68788	22.359	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.440%
11) 1,1-Dichloroethene-d2	4.013	63	192303	16.832	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.320%
21) 2-Butanone-d5	7.074	46	83313	50.039	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.080%
24) Chloroform-d	7.647	84	297754	23.701	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.305	65	158049	24.038	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.160%
32) Benzene-d6	8.275	84	624747	24.590	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.360%
36) 1,2-Dichloropropane-d6	9.268	67	191599	24.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.360%
41) Toluene-d8	10.323	98	558857	24.507	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.040%
43) trans-1,3-Dichloroprop...	10.573	79	71950	24.345	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.400%
47) 2-Hexanone-d5	10.921	63	62808	48.074	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.140%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	144415	23.764	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.040%
66) 1,2-Dichlorobenzene-d4	13.847	152	166823	24.818	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5887	0.593	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
Data File : VW024916.D
Acq On : 14 Oct 2022 09:01
Operator : SY/VA
Sample : VW1014SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 15 00:15:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 15 00:14:44 2022
Response via : Initial Calibration

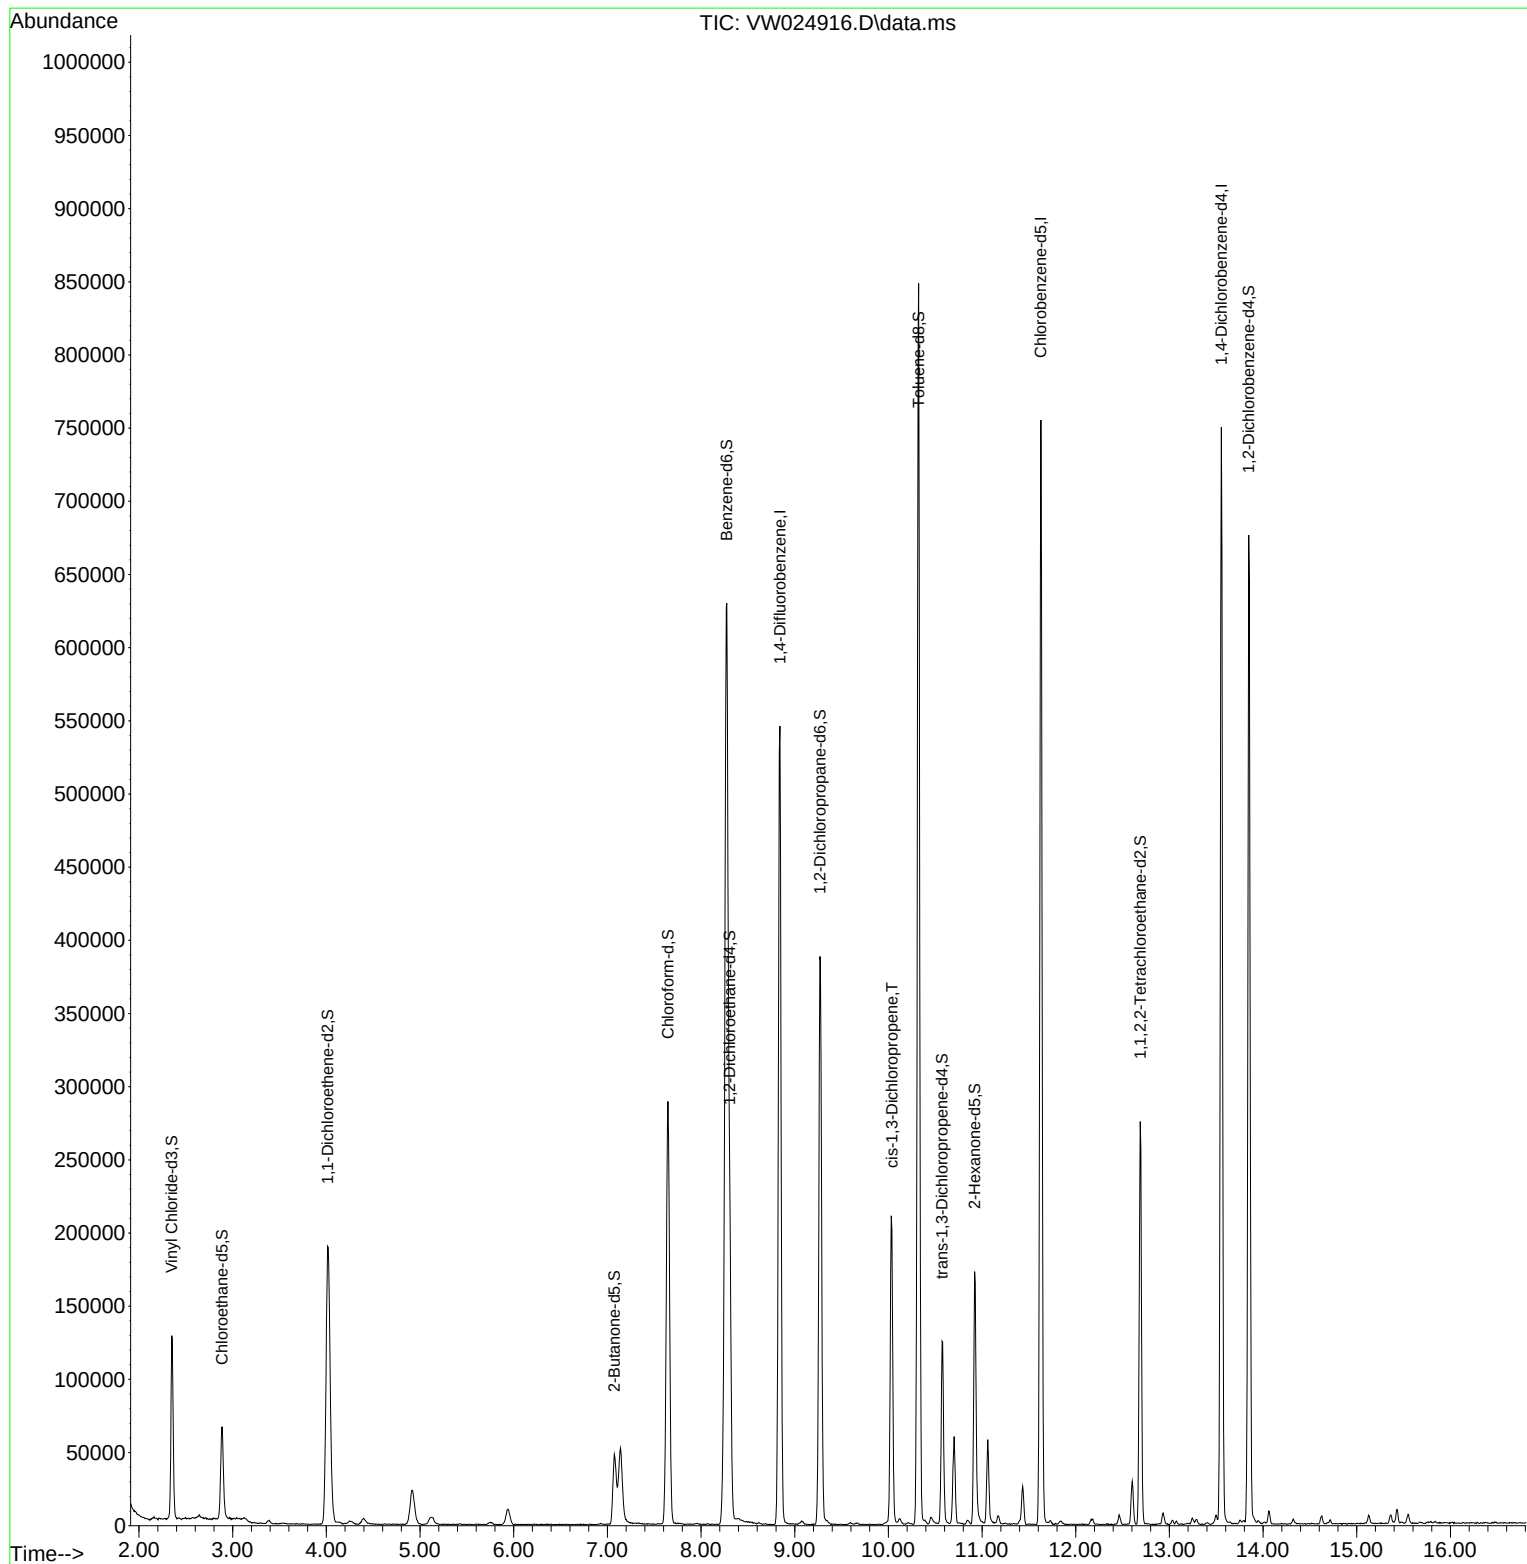

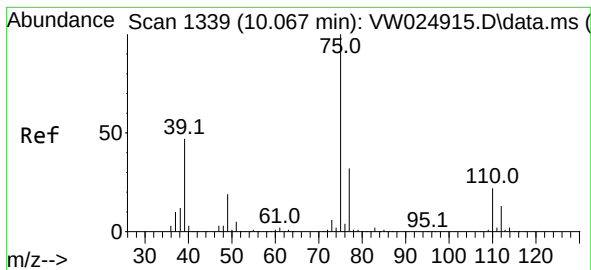

#39
 cis-1,3-Dichloropropene
 Concen: 0.593 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW024916.D
 Acq: 14 Oct 2022 09:01

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5887
 Ion Ratio Lower Upper
 75 100
 77 46.9 21.9 40.7#

