

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
 Data File : VW024918.D
 Acq On : 14 Oct 2022 09:50
 Operator : SY/VA
 Sample : N5023-08
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 15 00:15:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 15 00:14:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	459276	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	418945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	197578	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	118464	21.863	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.440%
7) Chloroethane-d5	2.885	69	70176	22.121	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.480%
11) 1,1-Dichloroethene-d2	4.147	63	190	0.016	ug/L	0.12
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.080%#
21) 2-Butanone-d5	7.080	46	82889	48.281	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.560%
24) Chloroform-d	7.647	84	292560	22.584	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.320%
26) 1,2-Dichloroethane-d4	8.470	65	114	0.017	ug/L	0.16
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.275	84	615359	23.423	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.680%
36) 1,2-Dichloropropane-d6	9.274	67	186279	23.118	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.480%
41) Toluene-d8	10.323	98	538858	22.853	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	10.579	79	69453	22.727	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.920%
47) 2-Hexanone-d5	10.920	63	65536	48.512	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.020%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	145901	23.218	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	164022	22.717	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5385	0.524	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
Data File : VW024918.D
Acq On : 14 Oct 2022 09:50
Operator : SY/VA
Sample : N5023-08
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 15 00:15:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 15 00:14:44 2022
Response via : Initial Calibration

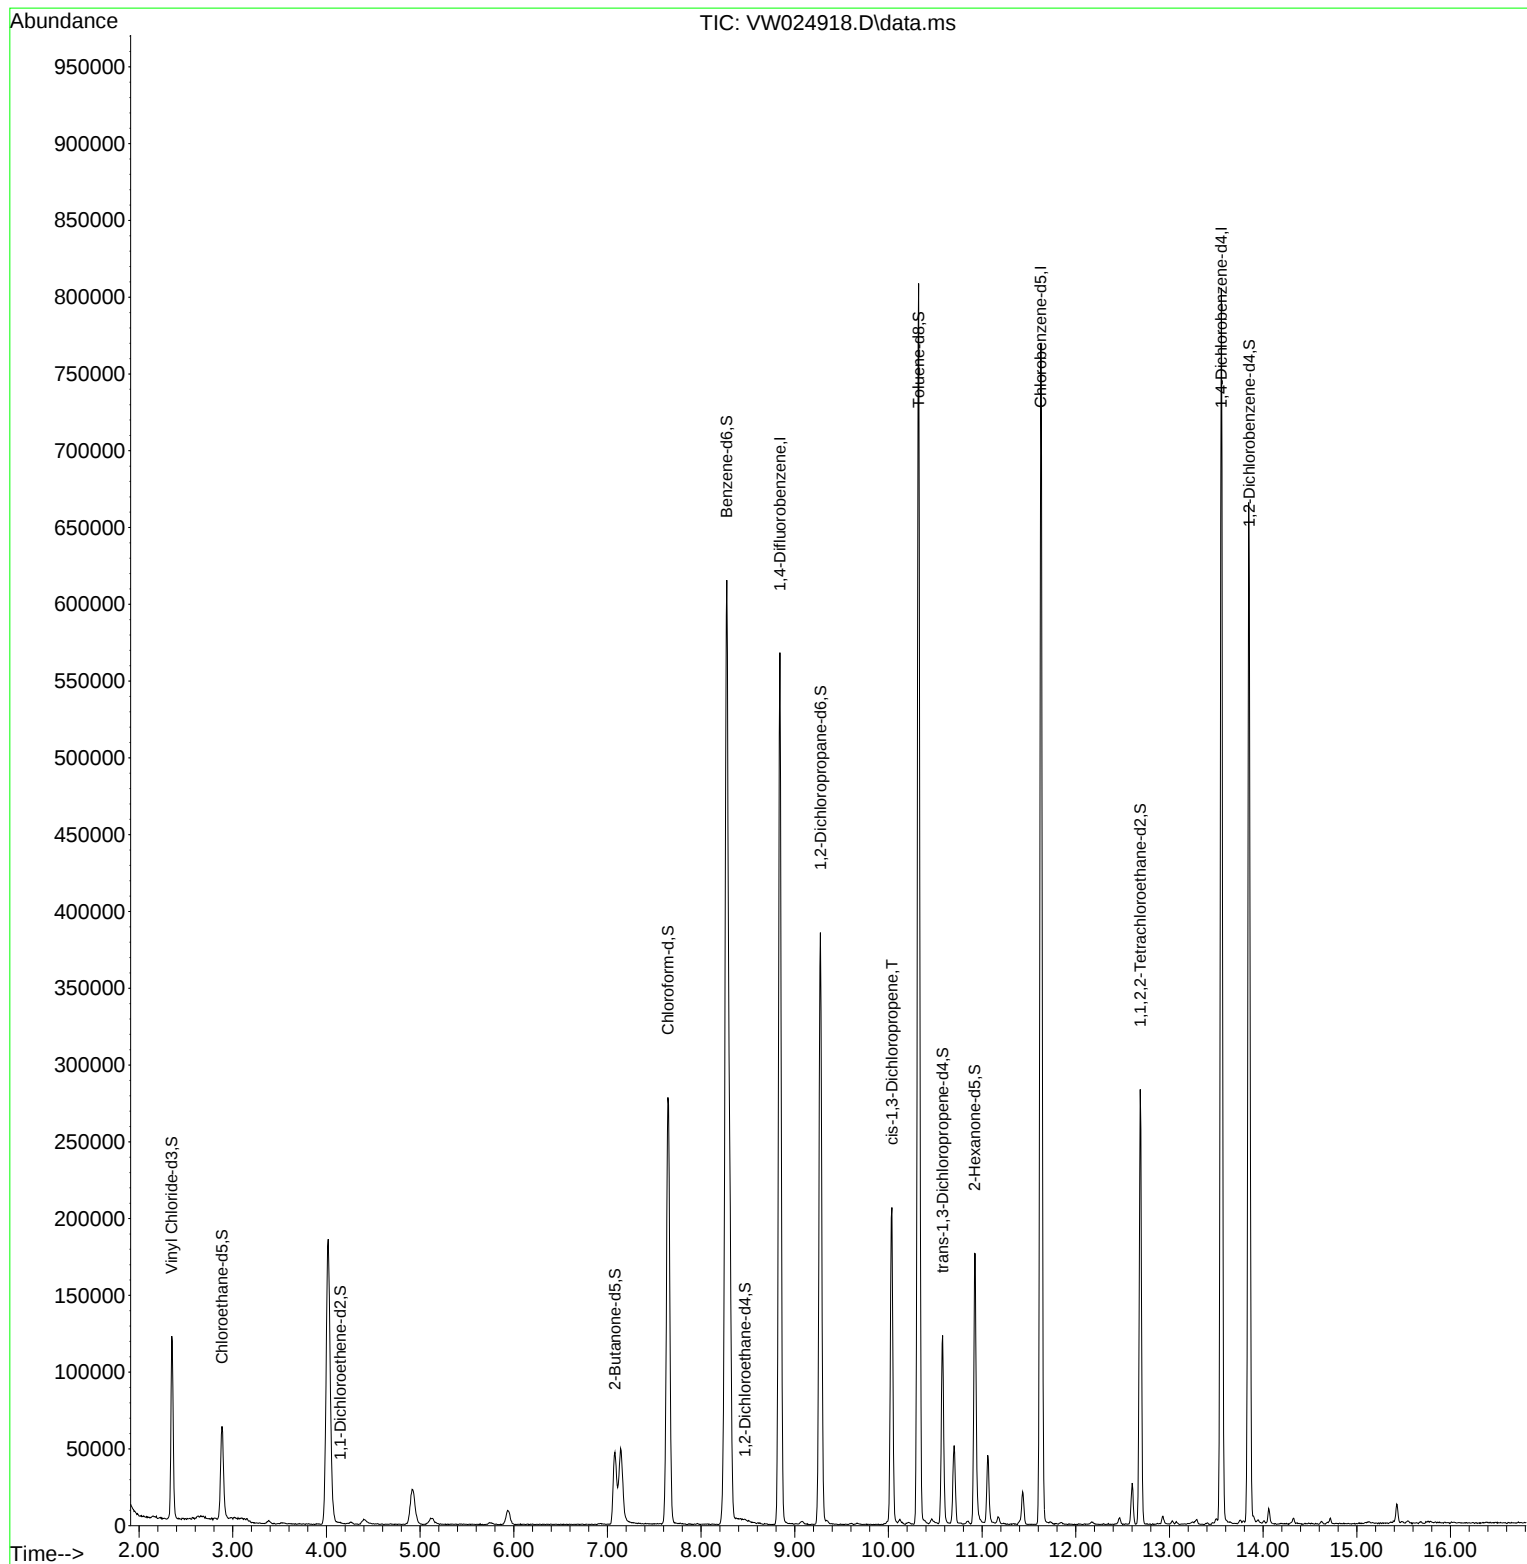

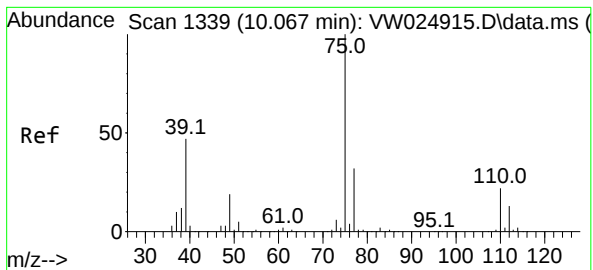

#39
 cis-1,3-Dichloropropene
 Concen: 0.524 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VW024918.D
 Acq: 14 Oct 2022 09:50

Instrument :
 MSVOA_W
 ClientSampleId :

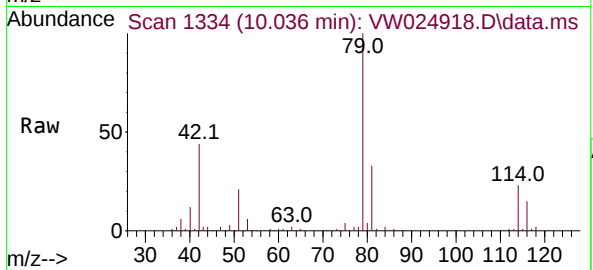

Tgt Ion: 75 Resp: 5385
 Ion Ratio Lower Upper
 75 100
 77 52.4 21.9 40.7#

