




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
 Data File : VW024922.D
 Acq On : 14 Oct 2022 11:27
 Operator : SY/VA
 Sample : N5049-11RE
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/15/2022
 Supervised By :Mahesh Dadoda 10/16/2022

Quant Time: Oct 15 00:16:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 15 00:14:44 2022
 Response via : Initial Calibration

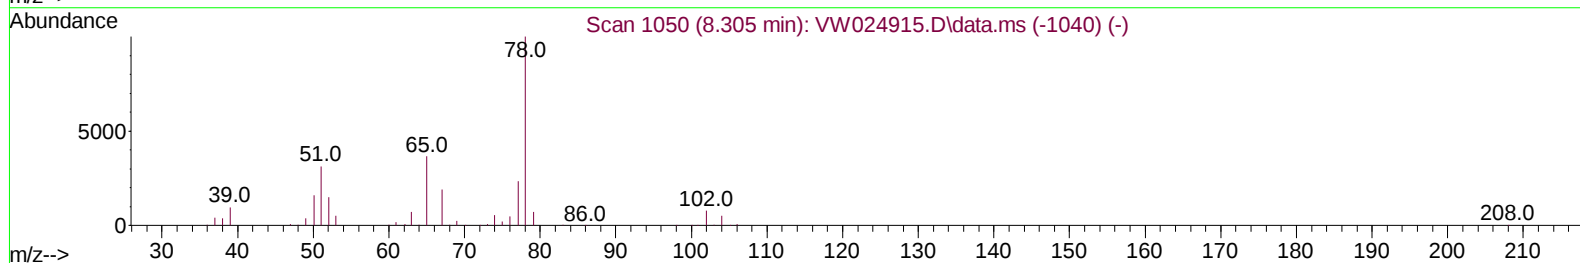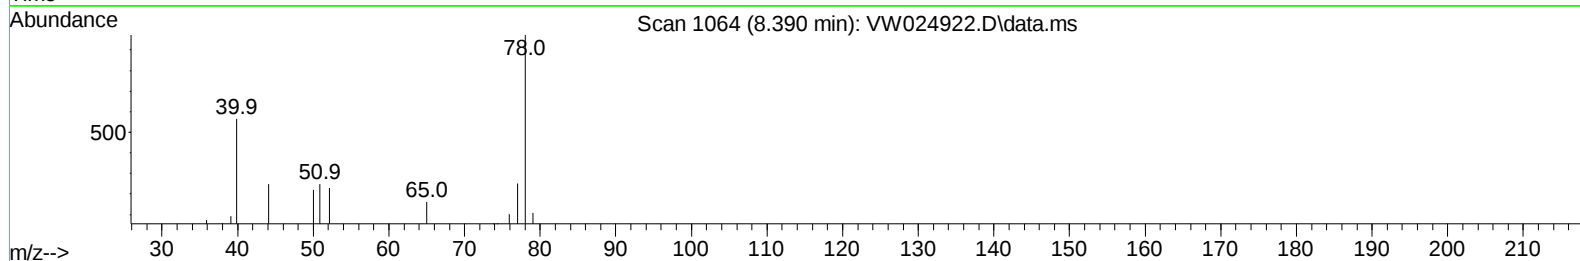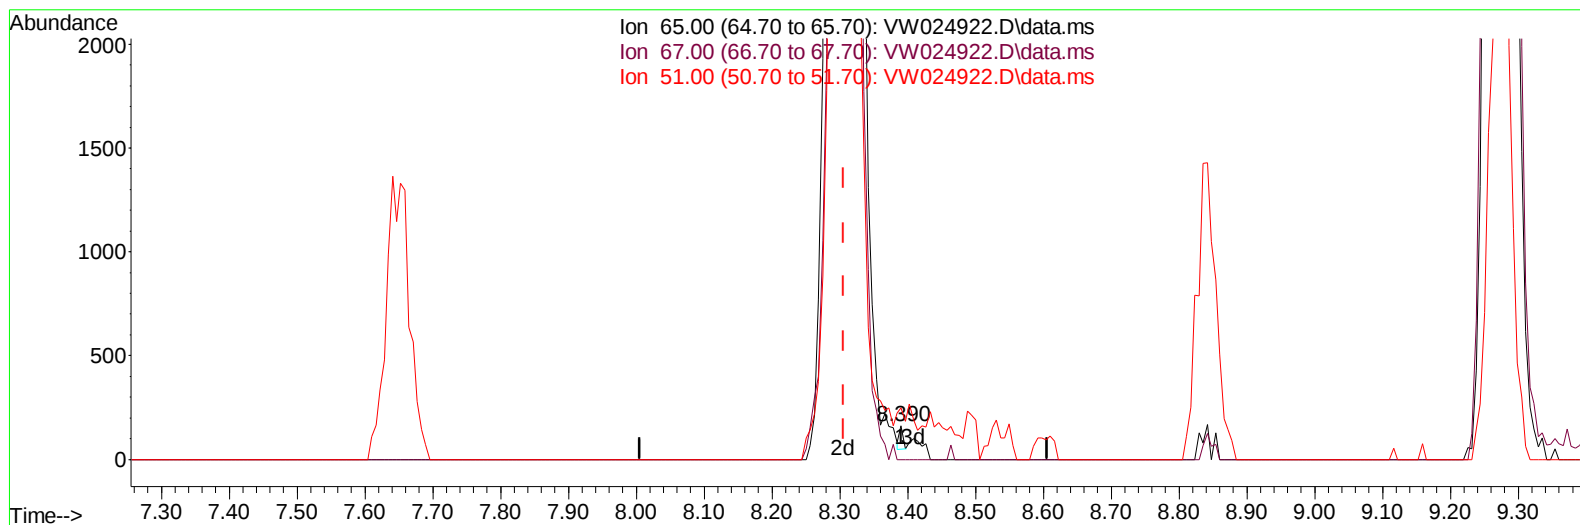

TIC: VW024922.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.390min (+ 0.085) 0.02 ug/L

response 41

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.90	63.41
51.00	120.80	151.22
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
 Data File : VW024922.D
 Acq On : 14 Oct 2022 11:27
 Operator : SY/VA
 Sample : N5049-11RE
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP7RE

Manual IntegrationsAPPROVED

Quant Time: Oct 15 00:16:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 15 00:14:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/15/2022
 Supervised By :Mahesh Dadoda 10/16/2022

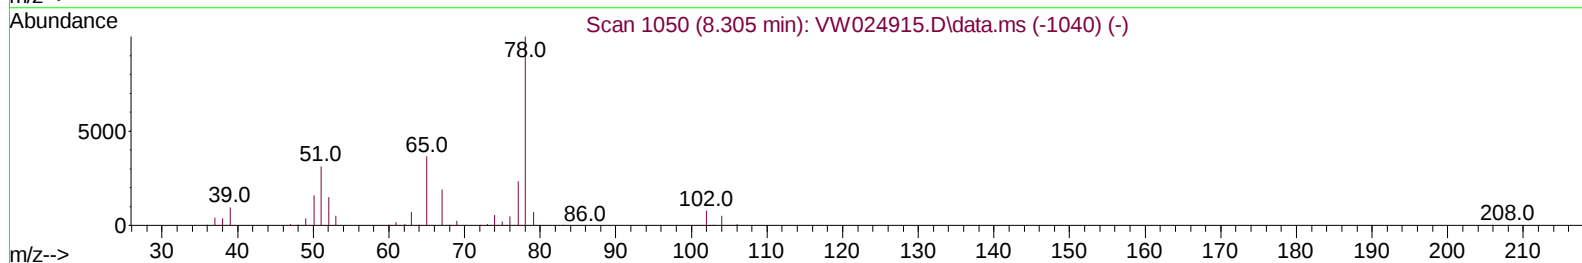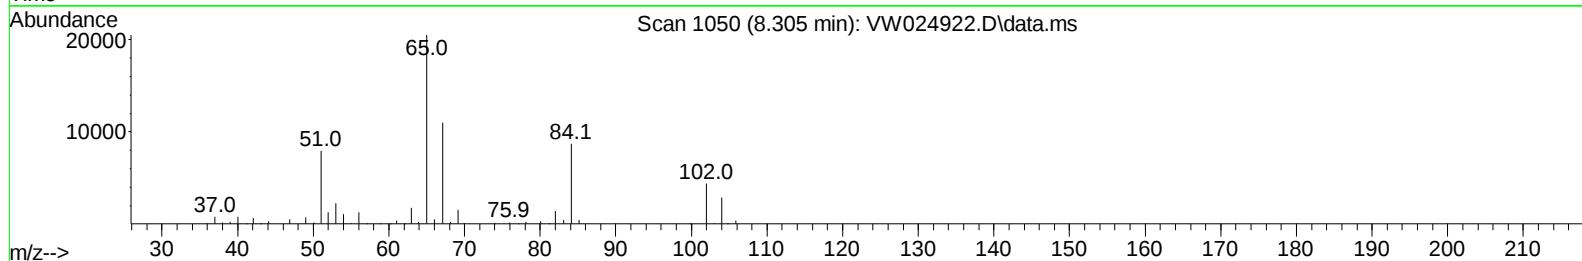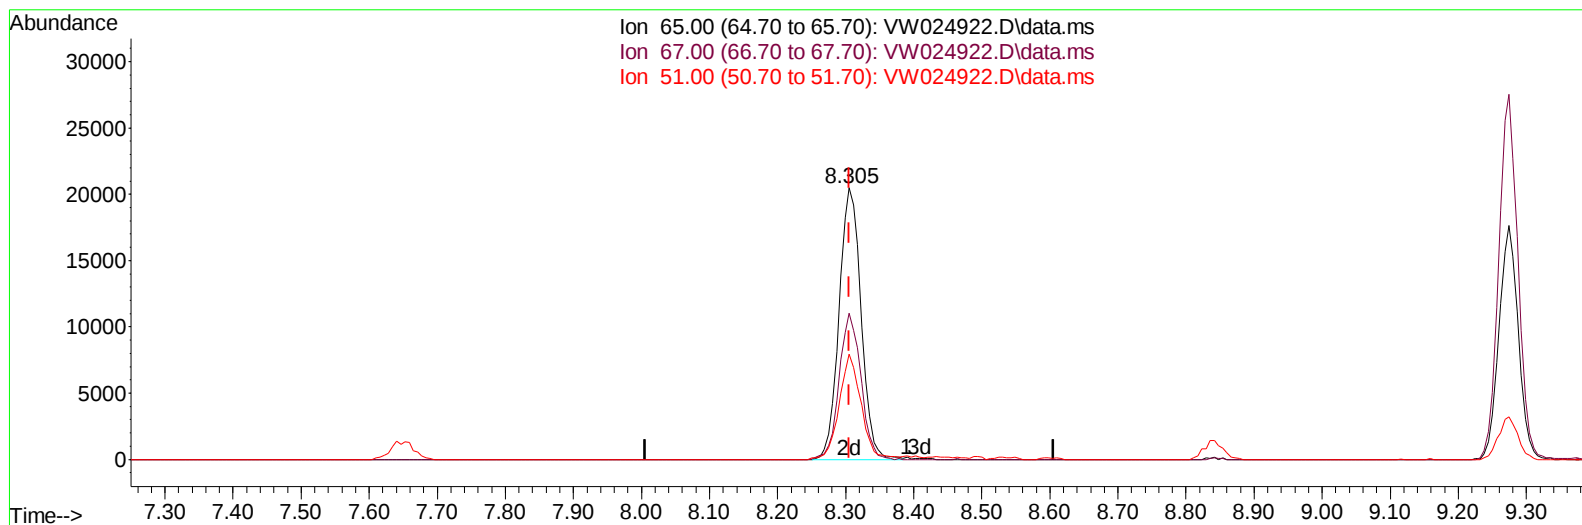

TIC: VW024922.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 21.75 ug/L m

response 45970

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.90	0.06#
51.00	120.80	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101422\
 Data File : VW024922.D
 Acq On : 14 Oct 2022 11:27
 Operator : SY/VA
 Sample : N5049-11RE
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/15/2022
 Supervised By :Mahesh Dadoda 10/16/2022

Quant Time: Oct 15 00:16:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 15 00:14:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	143189	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	113135	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	32630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	27905	16.519	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.080%		
7) Chloroethane-d5	2.885	69	20036	20.257	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.040%		
11) 1,1-Dichloroethene-d2	4.013	63	54089	14.726	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	58.920%		
21) 2-Butanone-d5	7.080	46	23049	43.062	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.120%		
24) Chloroform-d	7.653	84	86074	21.312	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.240%		
26) 1,2-Dichloroethane-d4	8.305	65	45970m	21.749	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.000%		
32) Benzene-d6	8.275	84	158538	22.347	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.400%		
36) 1,2-Dichloropropane-d6	9.274	67	54460	25.028	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.120%		
41) Toluene-d8	10.323	98	122992	19.315	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.280%		
43) trans-1,3-Dichloroprop...	10.579	79	16370	19.836	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.360%		
47) 2-Hexanone-d5	10.927	63	16140	44.242	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.480%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40167	23.670	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.680%		
66) 1,2-Dichlorobenzene-d4	13.847	152	25144	21.086	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.360%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101422\
Data File : VW024922.D
Acq On : 14 Oct 2022 11:27
Operator : SY/VA
Sample : N5049-11RE
Misc : 5.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/15/2022
Supervised By :Mahesh Dadoda 10/16/2022

Quant Time: Oct 15 00:16:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 15 00:14:44 2022
Response via : Initial Calibration

