

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
 Data File : VW030592.D
 Acq On : 14 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4350-10
 Misc : 6.18g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 15 01:11:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 15 01:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	543593	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	496989	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	222710	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	88785	10.391	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	41.560%
7) Chloroethane-d5	2.564	69	205	0.032	ug/L	-0.34
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.120%#
11) 1,1-Dichloroethene-d2	4.021	65	33529	9.435	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	37.720%#
21) 2-Butanone-d5	7.075	46	77875	50.644	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.280%
24) Chloroform-d	7.648	84	255214	16.417	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.680%
26) 1,2-Dichloroethane-d4	8.307	65	148259	18.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.360%
32) Benzene-d6	8.276	84	390242	13.529	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	54.120%
36) 1,2-Dichloropropane-d6	9.270	67	146976	17.360	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	69.440%#
41) Toluene-d8	10.325	98	325857	12.375	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	49.480%
43) trans-1,3-Dichloroprop...	10.575	79	60423	17.044	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.160%
47) 2-Hexanone-d5	10.922	63	65278	59.863	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	147390	23.705	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%
66) 1,2-Dichlorobenzene-d4	13.849	152	137096	18.193	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	72.760%#
Target Compounds						
13) Acetone	4.125	43	14941	6.637	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
Data File : VW030592.D
Acq On : 14 Oct 2024 16:43
Operator : SY/MD
Sample : P4350-10
Misc : 6.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 15 01:11:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 15 01:09:12 2024
Response via : Initial Calibration

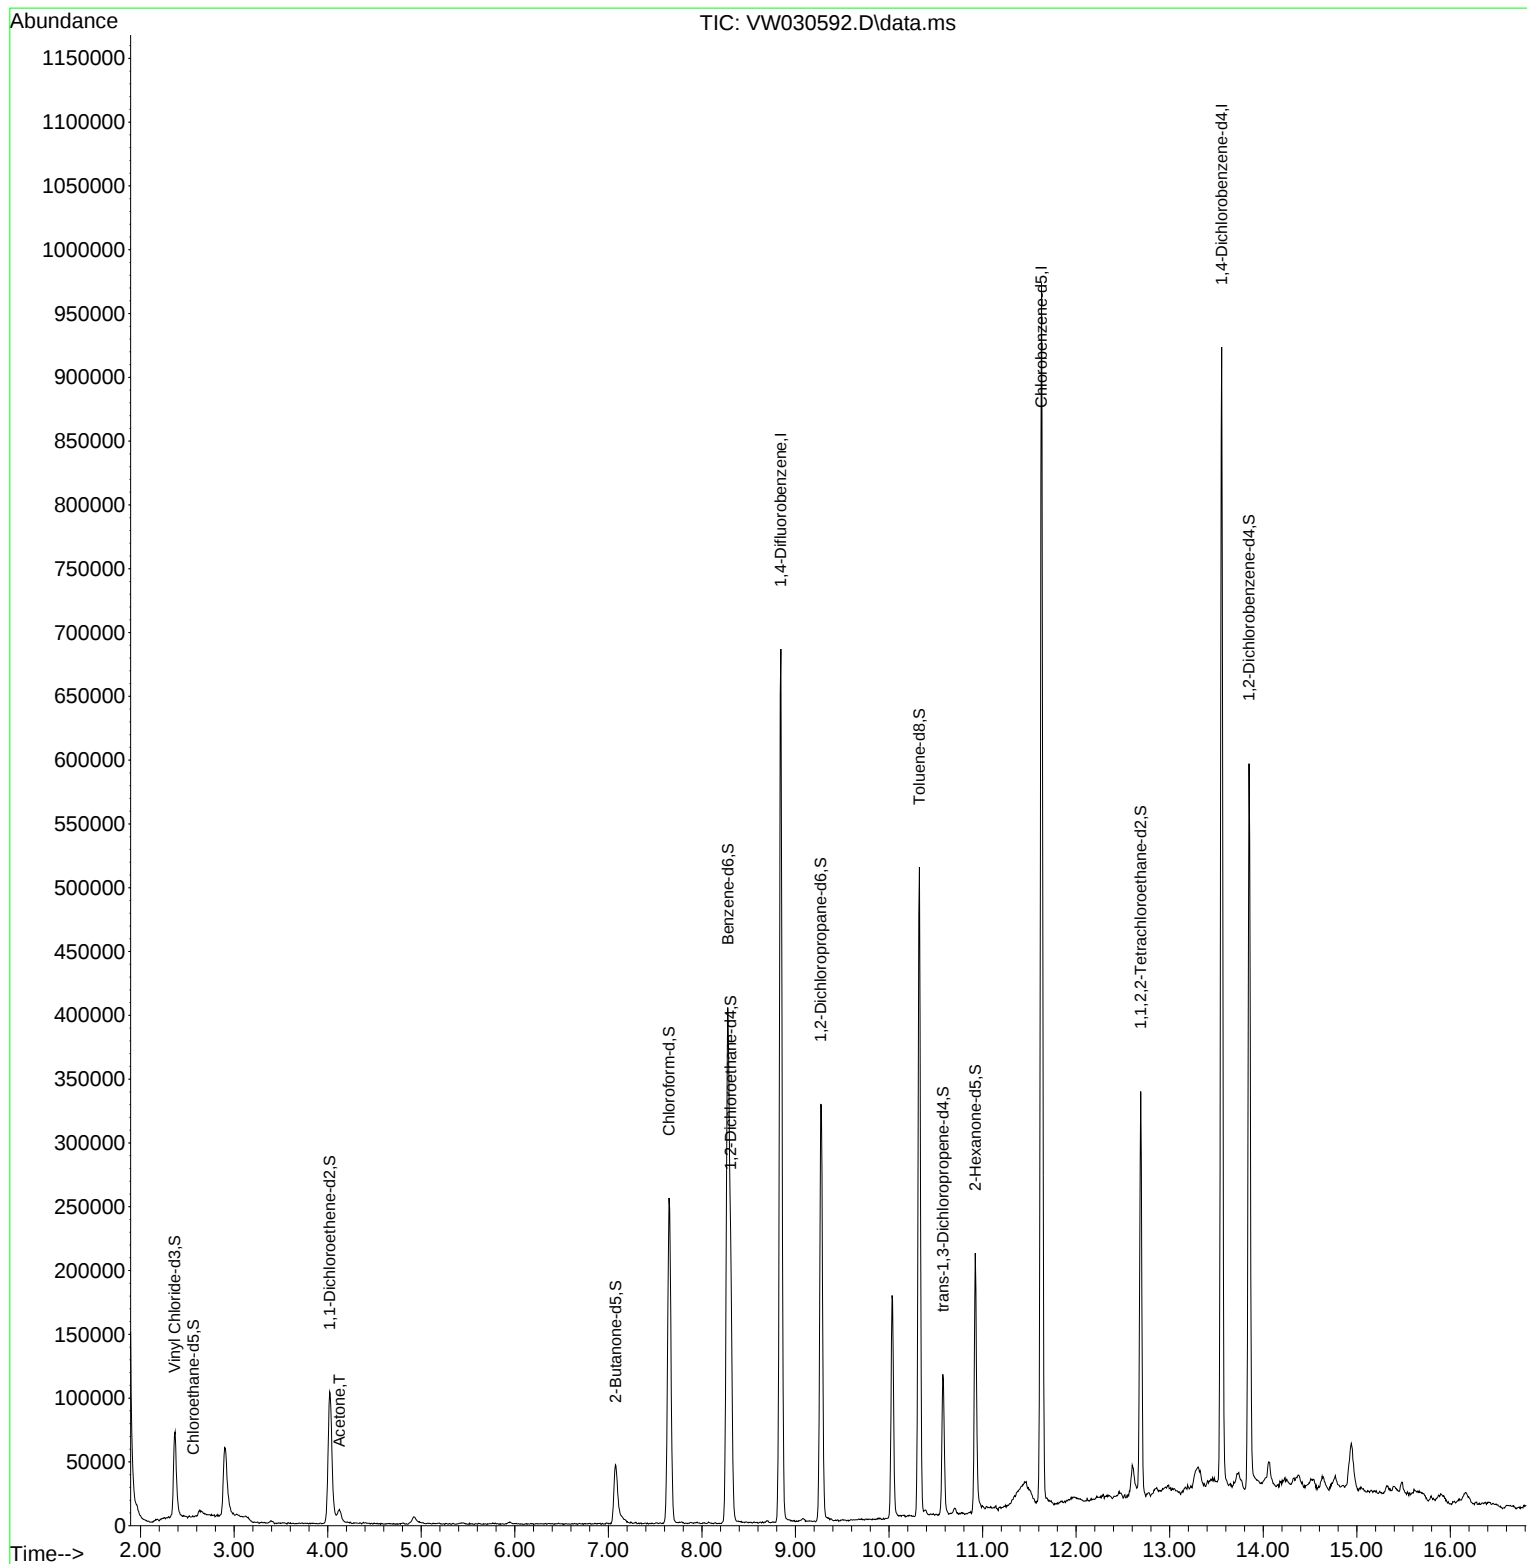

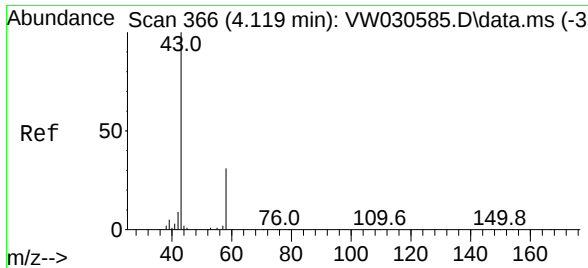

#13
 Acetone
 Concen: 6.637 ug/L
 RT: 4.125 min Scan# 3
 Delta R.T. 0.006 min
 Lab File: VW030592.D
 Acq: 14 Oct 2024 16:43

Instrument :
 MSVOA_W
 ClientSampleId :

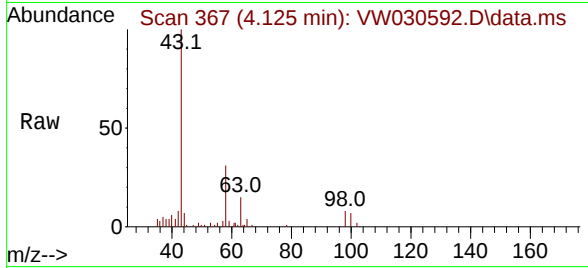

Tgt Ion: 43 Resp: 14941
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 57.6

