

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
 Data File : VW030593.D
 Acq On : 14 Oct 2024 17:07
 Operator : SY/MD
 Sample : P4350-09
 Misc : 6.56g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 15 01:11:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 15 01:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	60532	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	57621	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	26540	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	12249	12.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.480%
7) Chloroethane-d5	2.893	69	12017	16.685	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.760%
11) 1,1-Dichloroethene-d2	4.027	65	4801	12.132	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.520%
21) 2-Butanone-d5	7.203	46	236	1.378	ug/L	0.13
Spiked Amount	50.000	Range	20 - 135	Recovery	=	2.760%#
24) Chloroform-d	7.654	84	31246	18.050	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.200%
26) 1,2-Dichloroethane-d4	8.386	65	108	0.120	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.480%#
32) Benzene-d6	8.276	84	44982	13.450	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	53.800%
36) 1,2-Dichloropropane-d6	9.276	67	17190	17.512	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	70.040%
41) Toluene-d8	10.325	98	32897	10.775	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	43.120%
43) trans-1,3-Dichloroprop...	10.581	79	5377	13.082	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.320%
47) 2-Hexanone-d5	10.928	63	3617	28.609	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	16352	22.684	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.720%
66) 1,2-Dichlorobenzene-d4	13.849	152	15790	17.583	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	70.320%#
Target Compounds						
					Qvalue	
15) Methyl Acetate	4.667	43	98	0.316	ug/L #	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
Data File : VW030593.D
Acq On : 14 Oct 2024 17:07
Operator : SY/MD
Sample : P4350-09
Misc : 6.56g/10mL/MSVOA_W/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 15 01:11:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 15 01:09:12 2024
Response via : Initial Calibration

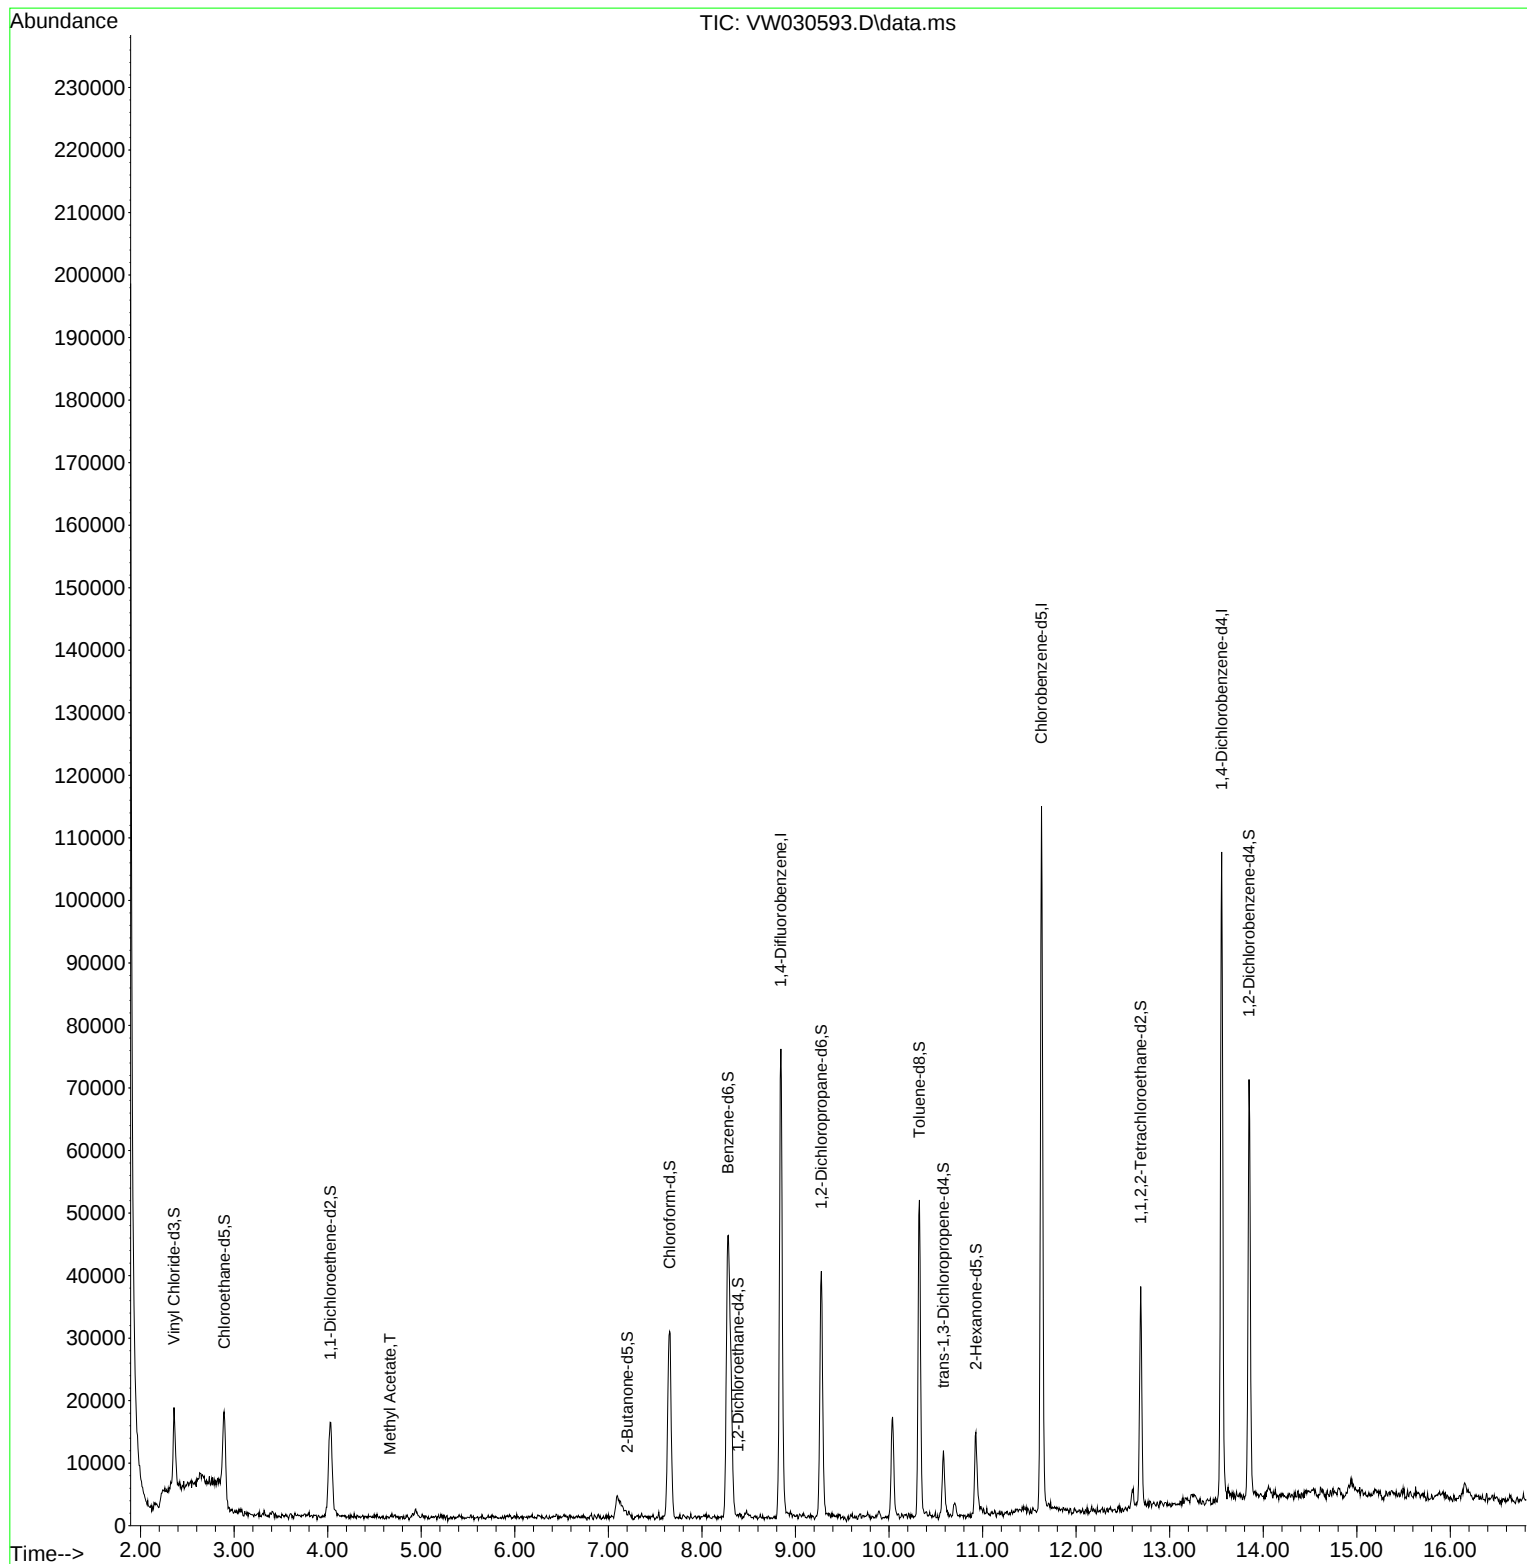

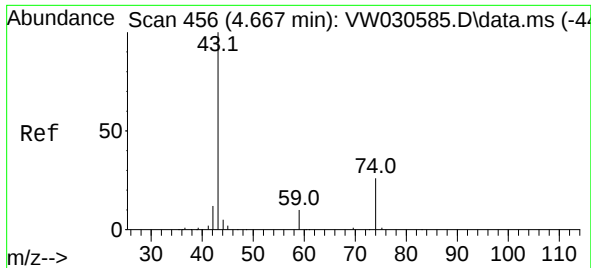

#15
Methyl Acetate
Concen: 0.316 ug/L
RT: 4.667 min Scan# 41
Delta R.T. 0.000 min
Lab File: VW030593.D
Acq: 14 Oct 2024 17:07

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 98
Ion Ratio Lower Upper
43 100
74 0.0 19.3 28.9#

