




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
Data File : VW030592.D
Acq On : 14 Oct 2024 16:43
Operator : SY/MD
Sample : P4350-10
Misc : 6.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAK0

Manual IntegrationsAPPROVED

Quant Time: Oct 15 01:11:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 15 01:09:12 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

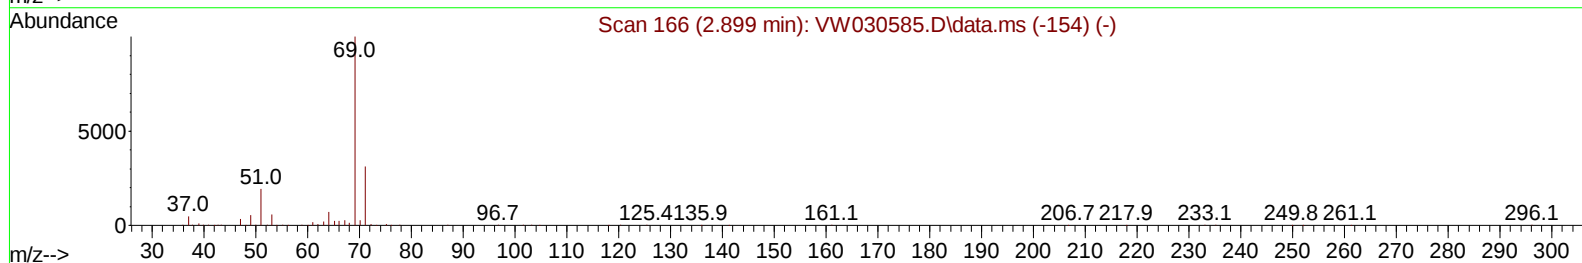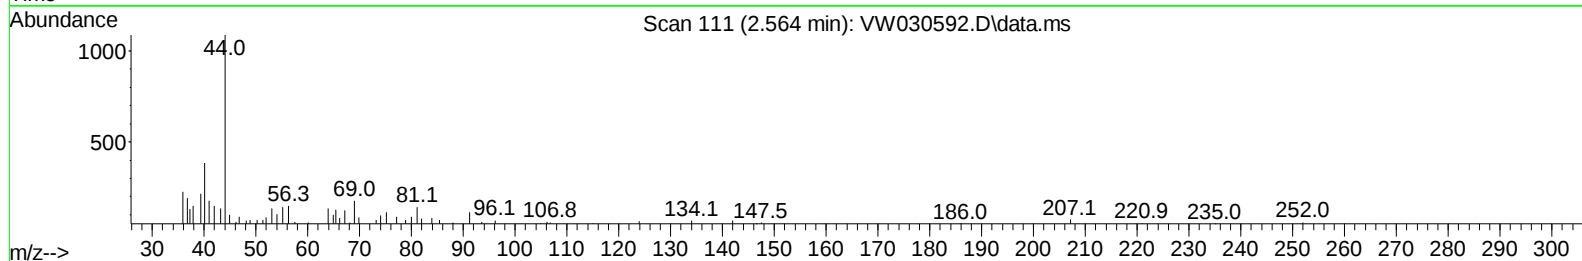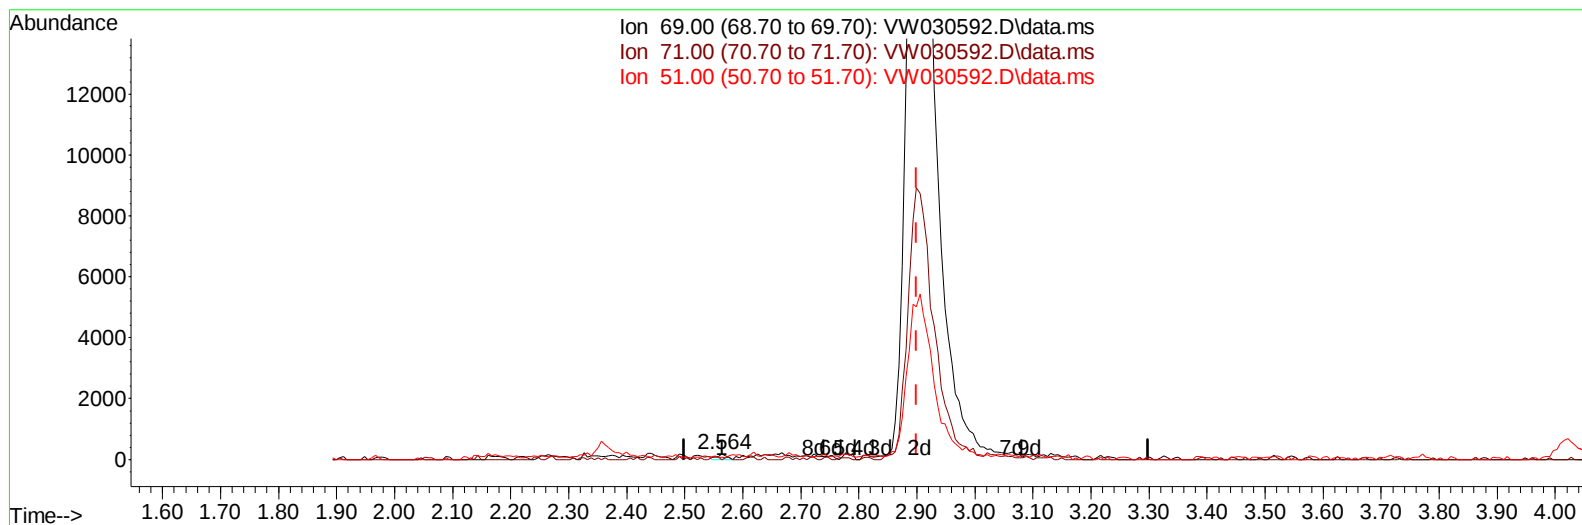

TIC: VW030592.D\data.ms

(7) Chloroethane-d5 (S)

2.564min (-0.335) 0.03 ug/L

response 205

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	40.49
51.00	10.20	10.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
 Data File : VW030592.D
 Acq On : 14 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4350-10
 Misc : 6.18g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK0

Manual IntegrationsAPPROVED

Quant Time: Oct 15 01:11:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 15 01:09:12 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

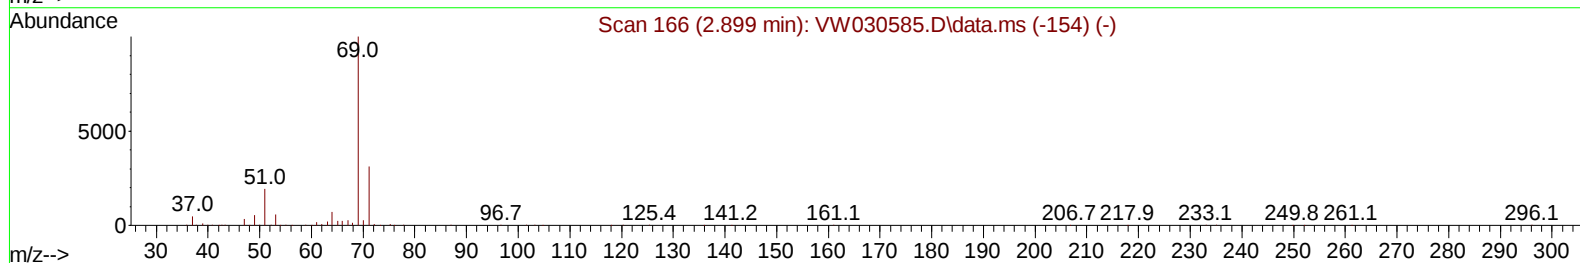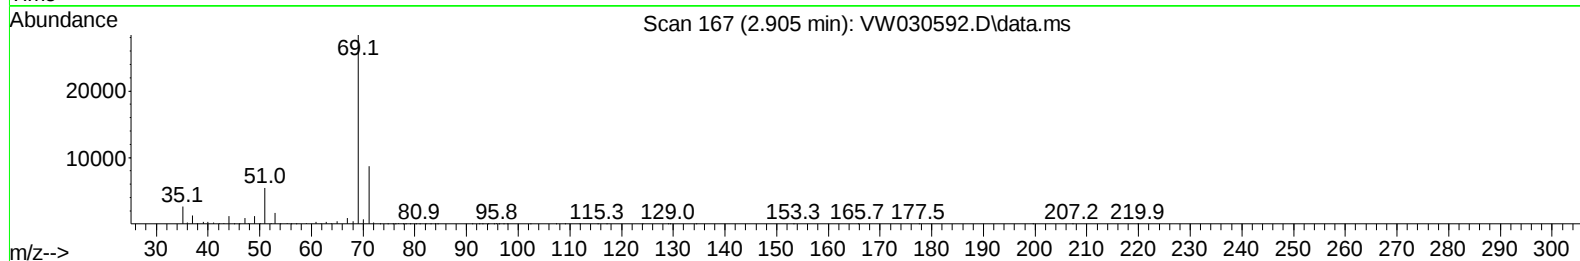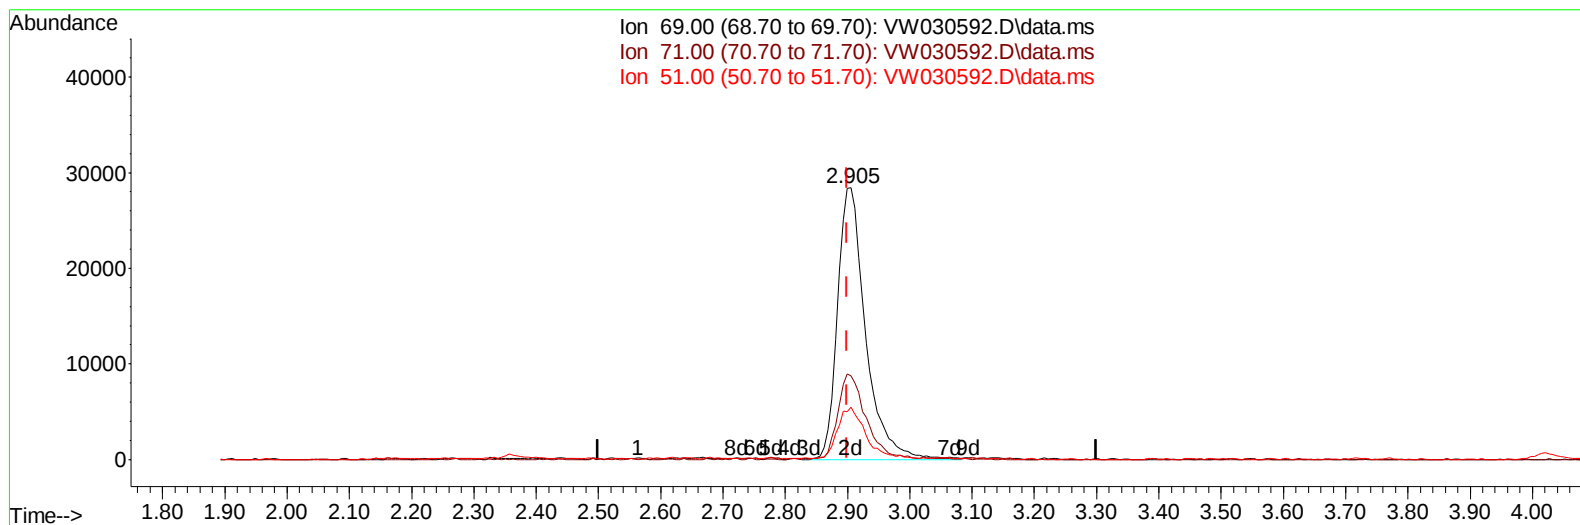

TIC: VW030592.D\data.ms

(7) Chloroethane-d5 (S)

2.905min (+ 0.006) 13.72 ug/L m

response 88736

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	0.09#
51.00	10.20	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101424\
 Data File : VW030592.D
 Acq On : 14 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4350-10
 Misc : 6.18g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK0

Manual IntegrationsAPPROVED

Quant Time: Oct 15 01:11:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 15 01:09:12 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		543593	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		496989	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		222710	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		88785	10.391	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	41.560%		
7) Chloroethane-d5	2.905	69		88736m	13.720	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.880%		
11) 1,1-Dichloroethene-d2	4.021	65		33529	9.435	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	37.720%#		
21) 2-Butanone-d5	7.075	46		77875	50.644	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.280%		
24) Chloroform-d	7.648	84		255214	16.417	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	65.680%		
26) 1,2-Dichloroethane-d4	8.307	65		148259	18.340	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	73.360%		
32) Benzene-d6	8.276	84		390242	13.529	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	54.120%		
36) 1,2-Dichloropropane-d6	9.270	67		146976	17.360	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	69.440%#		
41) Toluene-d8	10.325	98		325857	12.375	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	49.480%		
43) trans-1,3-Dichloroprop...	10.575	79		60423	17.044	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	68.160%		
47) 2-Hexanone-d5	10.922	63		65278	59.863	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	119.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		147390	23.705	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.840%		
66) 1,2-Dichlorobenzene-d4	13.849	152		137096	18.193	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	72.760%#		
Target Compounds							
13) Acetone	4.125	43		14941	6.637	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
Data File : VW030592.D
Acq On : 14 Oct 2024 16:43
Operator : SY/MD
Sample : P4350-10
Misc : 6.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAK0

Manual IntegrationsAPPROVED

Quant Time: Oct 15 01:11:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 15 01:09:12 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

