

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
 Data File : VW030592.D
 Acq On : 14 Oct 2024 16:43
 Operator : SY/MD
 Sample : P4350-10
 Misc : 6.18g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK0

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 15 01:11:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 15 01:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	543593	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	496989	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	222710	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	88785	10.391	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	41.560%		
7) Chloroethane-d5	2.905	69	88736m	13.720	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.880%		
11) 1,1-Dichloroethene-d2	4.021	65	33529	9.435	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	37.720%#		
21) 2-Butanone-d5	7.075	46	77875	50.644	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.280%		
24) Chloroform-d	7.648	84	255214	16.417	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	65.680%		
26) 1,2-Dichloroethane-d4	8.307	65	148259	18.340	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	73.360%		
32) Benzene-d6	8.276	84	390242	13.529	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	54.120%		
36) 1,2-Dichloropropane-d6	9.270	67	146976	17.360	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	69.440%#		
41) Toluene-d8	10.325	98	325857	12.375	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	49.480%		
43) trans-1,3-Dichloroprop...	10.575	79	60423	17.044	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	68.160%		
47) 2-Hexanone-d5	10.922	63	65278	59.863	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	119.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	147390	23.705	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.840%		
66) 1,2-Dichlorobenzene-d4	13.849	152	137096	18.193	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	72.760%#		
Target Compounds					Qvalue	
13) Acetone	4.125	43	14941	6.637	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101424\
Data File : VW030592.D
Acq On : 14 Oct 2024 16:43
Operator : SY/MD
Sample : P4350-10
Misc : 6.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAK0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024


Quant Time: Oct 15 01:11:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 15 01:09:12 2024
Response via : Initial Calibration

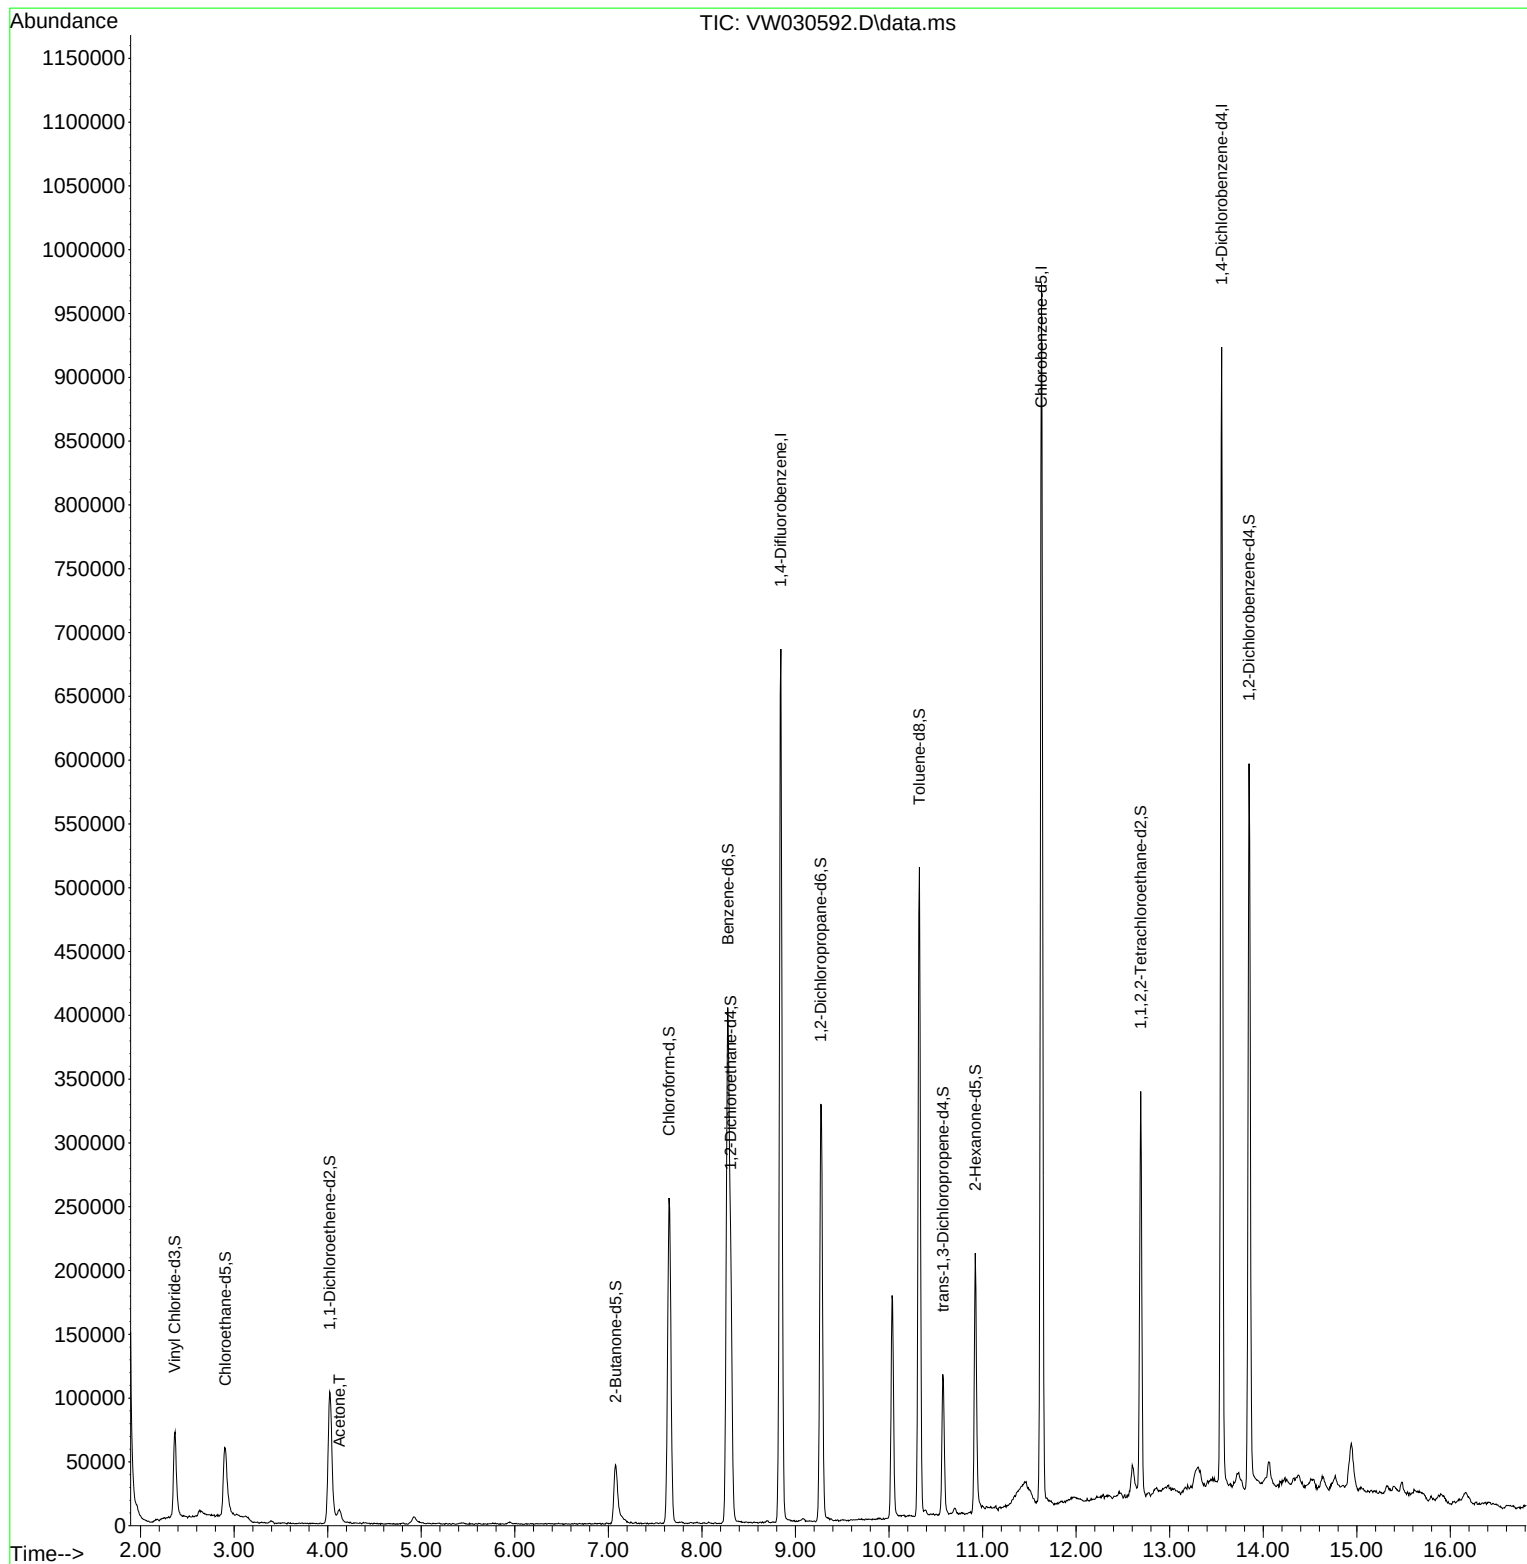

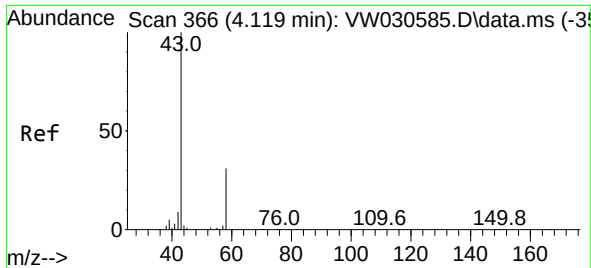

#13
 Acetone
 Concen: 6.637 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030592.D
 Acq: 14 Oct 2024 16:43

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAK0

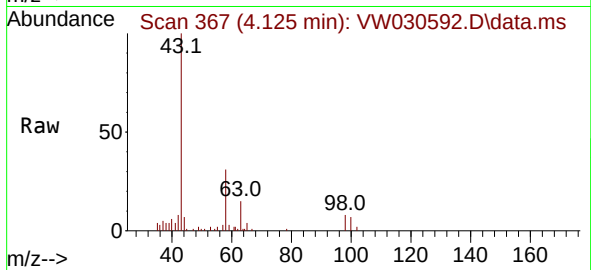

Tgt Ion: 43 Resp: 1494
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

