

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101524\
 Data File : VW030603.D
 Acq On : 15 Oct 2024 13:21
 Operator : SY/MD
 Sample : P4361-15
 Misc : 5.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 16 01:30:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 16 01:28:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	278037	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	267852	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	119044	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	77089	17.639	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.560%
7) Chloroethane-d5	2.899	69	69644	21.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.200%
11) 1,1-Dichloroethene-d2	4.021	65	32832	18.062	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.240%
21) 2-Butanone-d5	7.075	46	40181	51.089	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.180%
24) Chloroform-d	7.648	84	168383	21.177	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.720%
26) 1,2-Dichloroethane-d4	8.307	65	94480	22.851	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	8.276	84	305566	19.655	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.640%
36) 1,2-Dichloropropane-d6	9.270	67	95513	20.932	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.720%
41) Toluene-d8	10.325	98	269262	18.973	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.880%
43) trans-1,3-Dichloroprop...	10.575	79	39000	20.412	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.640%
47) 2-Hexanone-d5	10.922	63	29171	49.636	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	80163	23.922	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	93208	23.140	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.560%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3194	0.486	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101524\
Data File : VW030603.D
Acq On : 15 Oct 2024 13:21
Operator : SY/MD
Sample : P4361-15
Misc : 5.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 16 01:30:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 16 01:28:14 2024
Response via : Initial Calibration

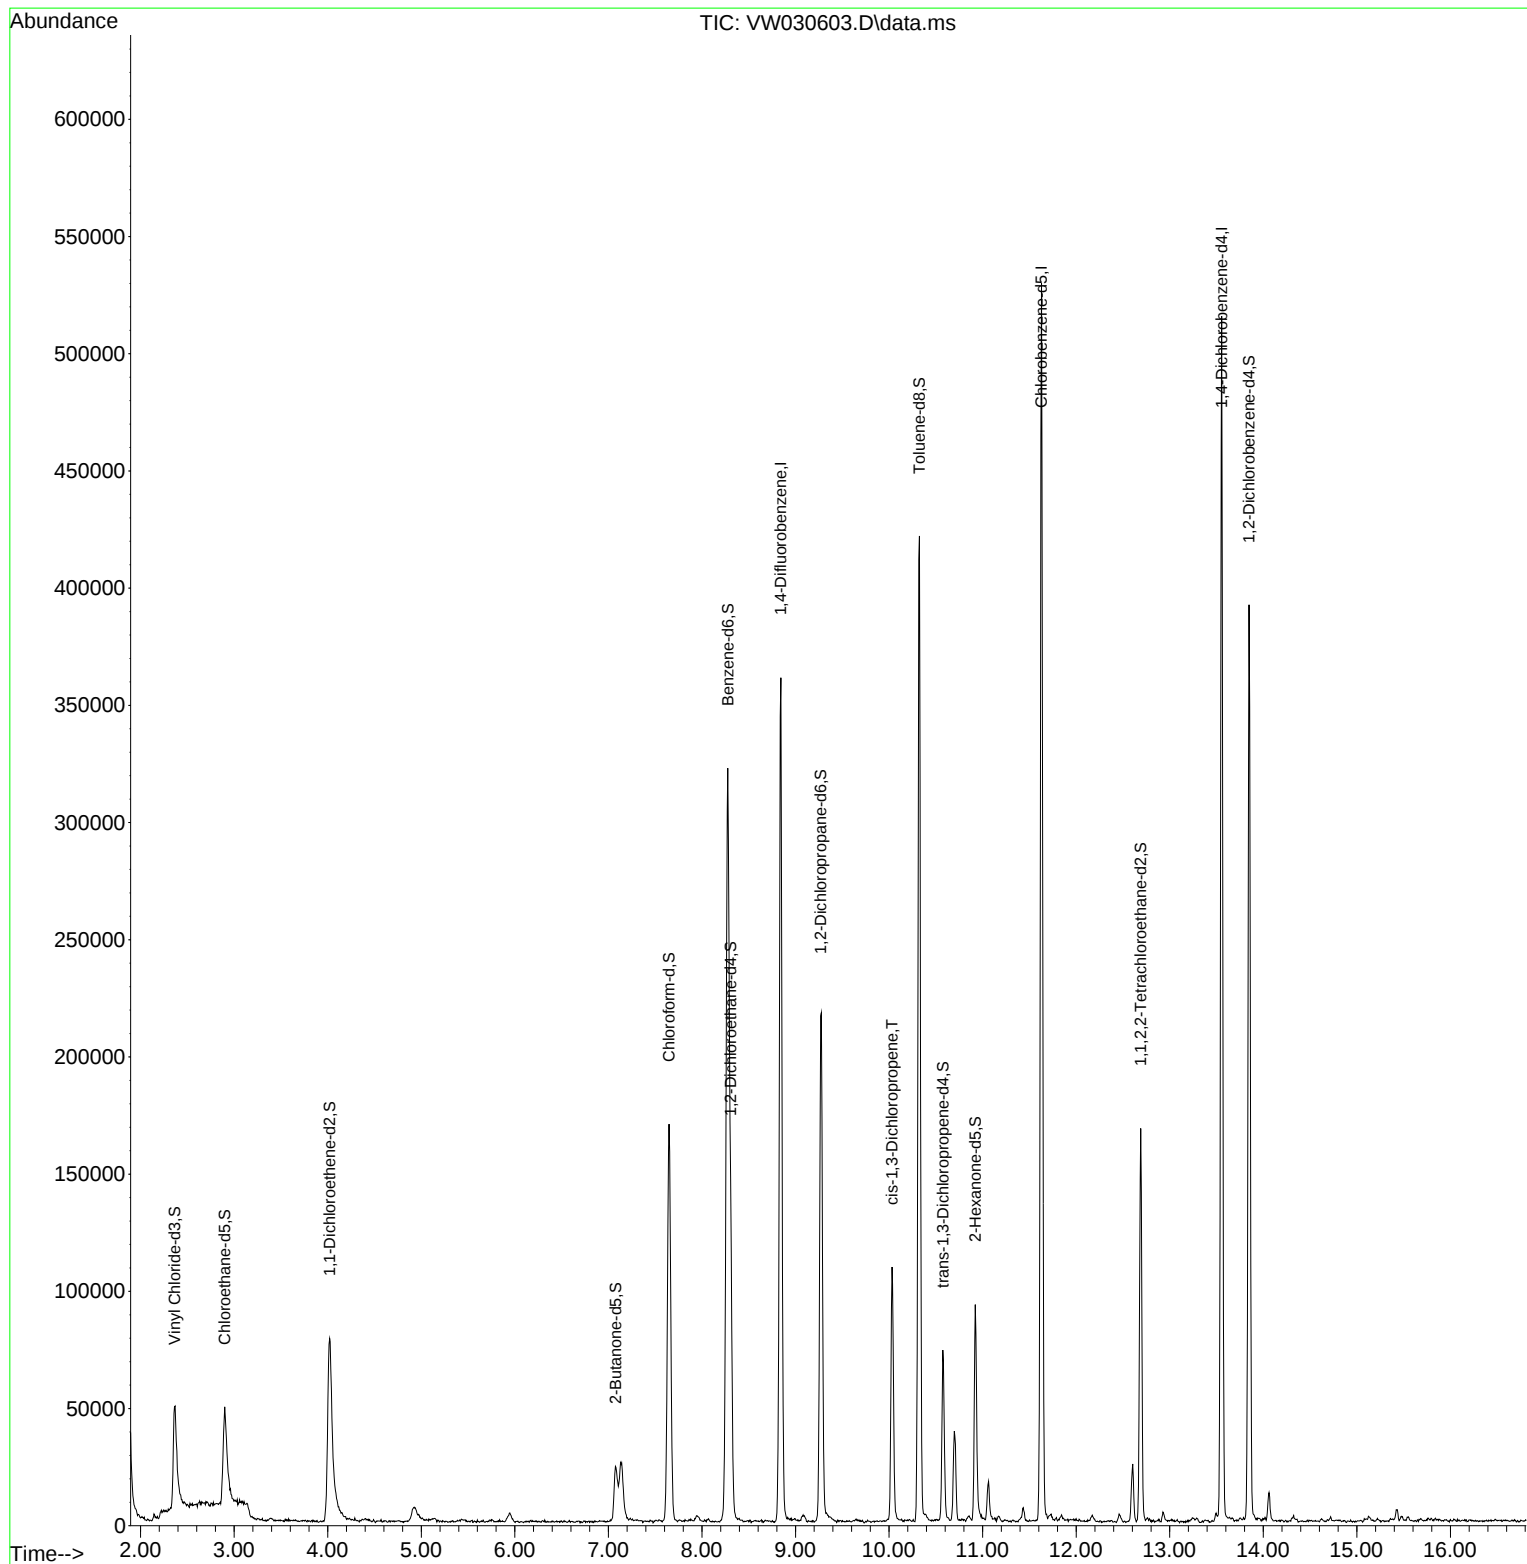

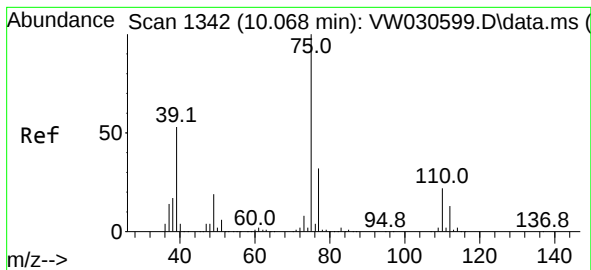

#39
 cis-1,3-Dichloropropene
 Concen: 0.486 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW030603.D
 Acq: 15 Oct 2024 13:21

Instrument :
 MSVOA_W
 ClientSampleId :

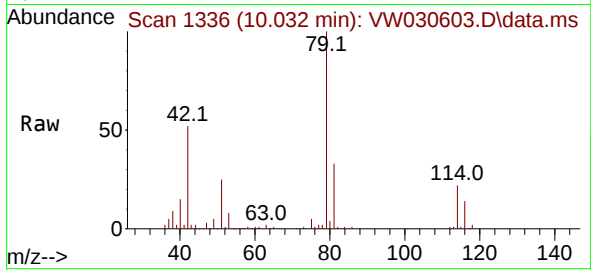

Tgt Ion: 75 Resp: 3194
 Ion Ratio Lower Upper
 75 100
 77 47.0 21.1 39.1#

