

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101524\
 Data File : VW030606.D
 Acq On : 15 Oct 2024 14:34
 Operator : SY/MD
 Sample : P4346-21
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 16 01:31:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 16 01:28:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	271068	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	255946	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	117748	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	86025	20.190	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.760%		
7) Chloroethane-d5	2.899	69	78022	24.191	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.760%		
11) 1,1-Dichloroethene-d2	4.021	65	36311	20.490	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	81.960%		
21) 2-Butanone-d5	7.081	46	46729	60.942	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	121.880%		
24) Chloroform-d	7.648	84	192093	24.780	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.120%		
26) 1,2-Dichloroethane-d4	8.301	65	107021	26.549	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	106.200%		
32) Benzene-d6	8.276	84	351208	23.642	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.560%		
36) 1,2-Dichloropropane-d6	9.276	67	109989	25.226	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.920%		
41) Toluene-d8	10.319	98	309467	22.820	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.280%		
43) trans-1,3-Dichloroprop...	10.575	79	43732	23.953	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.800%		
47) 2-Hexanone-d5	10.922	63	35216	62.709	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	125.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94238	29.431	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	117.720%		
66) 1,2-Dichlorobenzene-d4	13.848	152	106991	26.854	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.400%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4143	0.660	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101524\
Data File : VW030606.D
Acq On : 15 Oct 2024 14:34
Operator : SY/MD
Sample : P4346-21
Misc : 5.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 16 01:31:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 16 01:28:14 2024
Response via : Initial Calibration

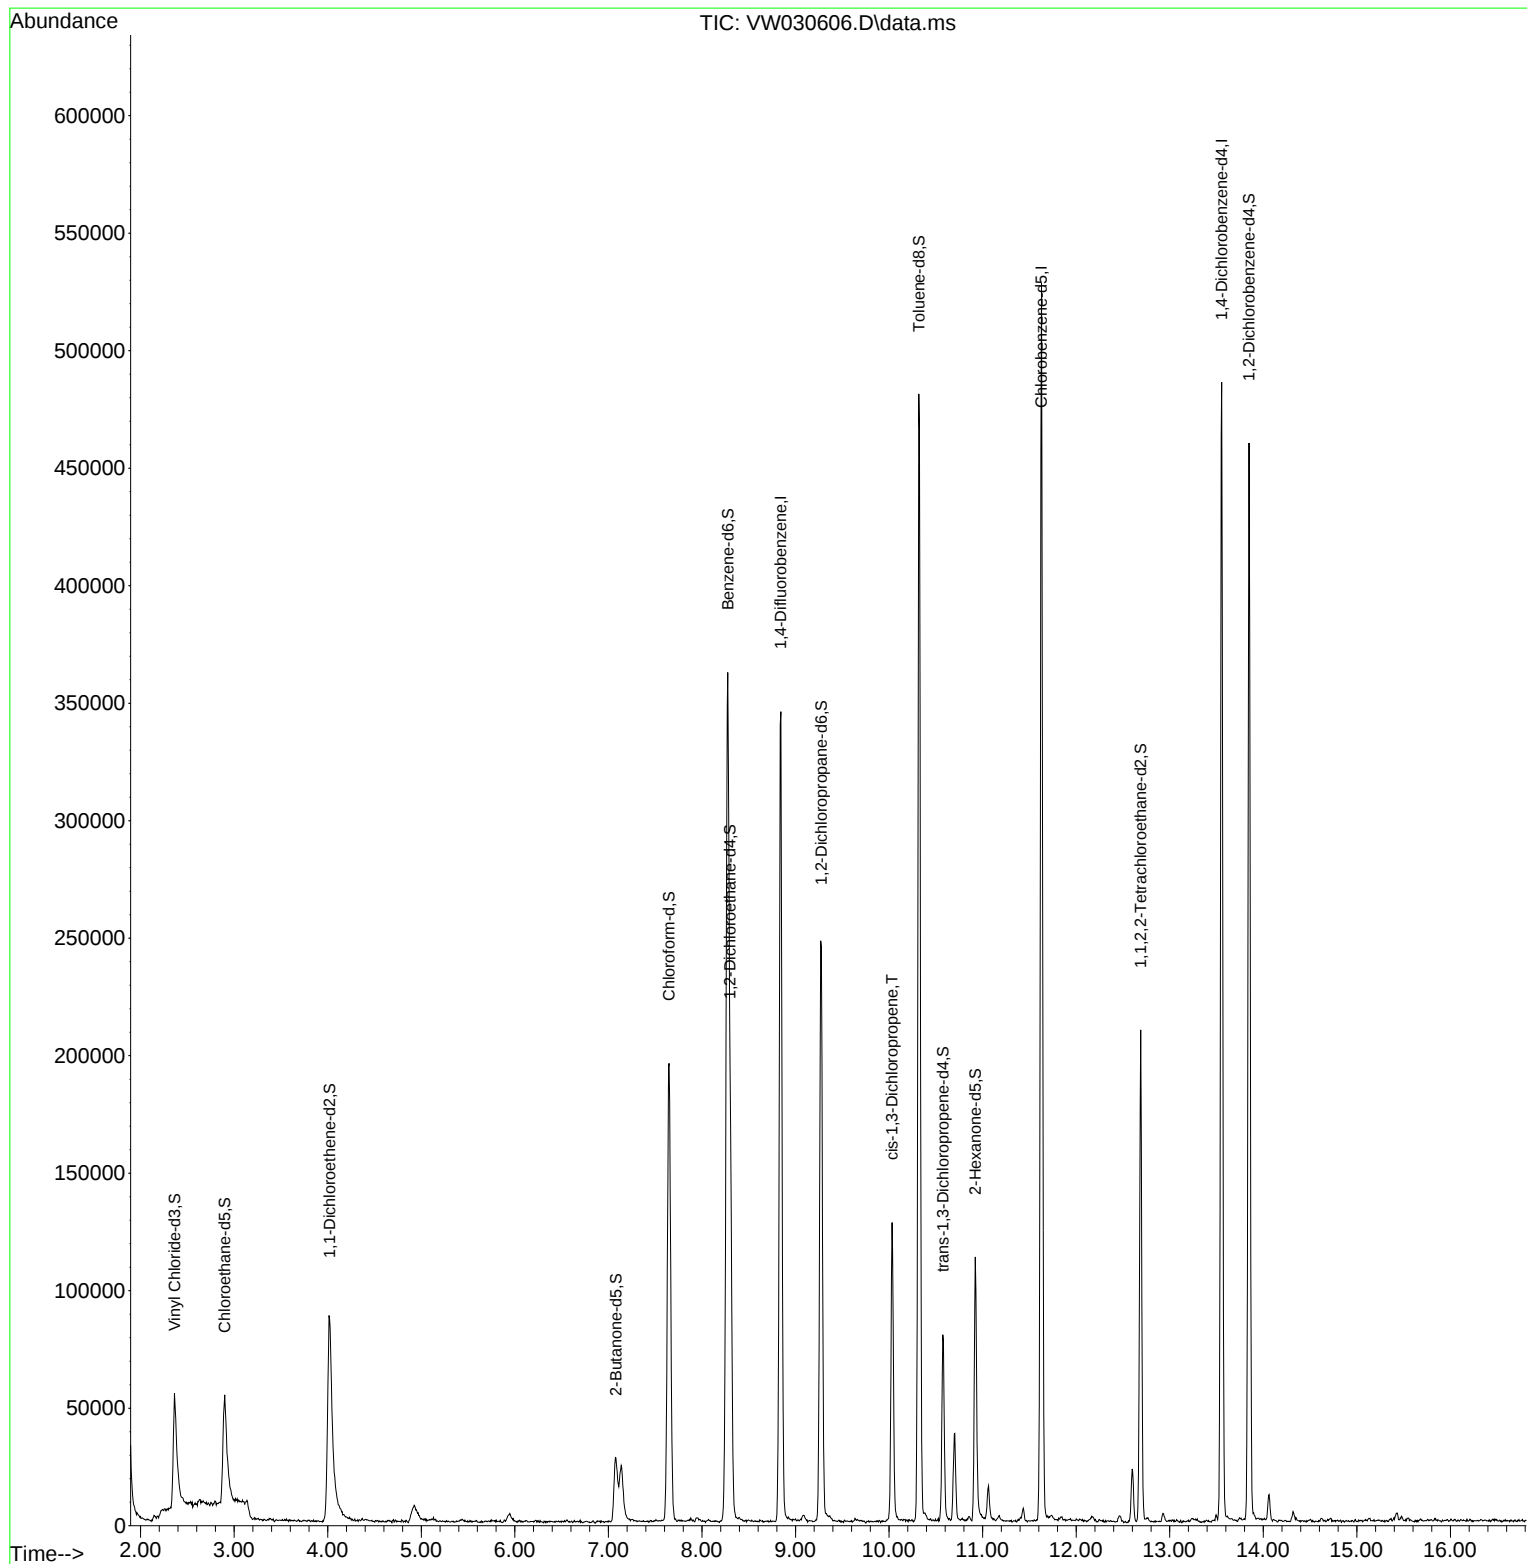

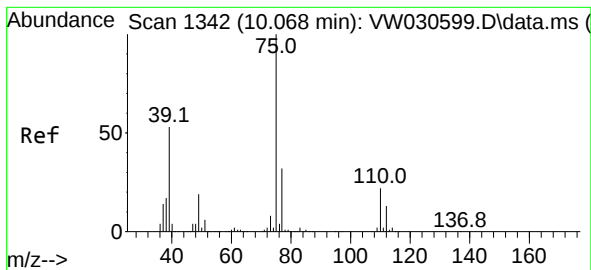

#39
 cis-1,3-Dichloropropene
 Concen: 0.660 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030606.D
 Acq: 15 Oct 2024 14:34

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4143
 Ion Ratio Lower Upper
 75 100
 77 48.6 21.1 39.1#

