

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101624\
 Data File : VW030613.D
 Acq On : 16 Oct 2024 15:58
 Operator : SY/MD
 Sample : VW1016SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 17 01:54:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 17 01:53:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	237315	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	233055	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	97820	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	69037	18.507	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.040%
7) Chloroethane-d5	2.893	69	63156	22.367	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.480%
11) 1,1-Dichloroethene-d2	4.021	65	25140	16.204	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.800%
21) 2-Butanone-d5	7.075	46	30194	44.978	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.960%
24) Chloroform-d	7.648	84	142832	21.046	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.200%
26) 1,2-Dichloroethane-d4	8.307	65	78973	22.378	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.520%
32) Benzene-d6	8.270	84	255576	18.894	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.560%
36) 1,2-Dichloropropane-d6	9.270	67	80979	20.397	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.600%
41) Toluene-d8	10.325	98	223026	18.062	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.240%
43) trans-1,3-Dichloroprop...	10.575	79	30224	18.180	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.720%
47) 2-Hexanone-d5	10.922	63	22020	43.062	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66686	22.872	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	74890	22.627	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2839	0.497	ug/L	# 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101624\
Data File : VW030613.D
Acq On : 16 Oct 2024 15:58
Operator : SY/MD
Sample : VW1016SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 17 01:54:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 17 01:53:12 2024
Response via : Initial Calibration

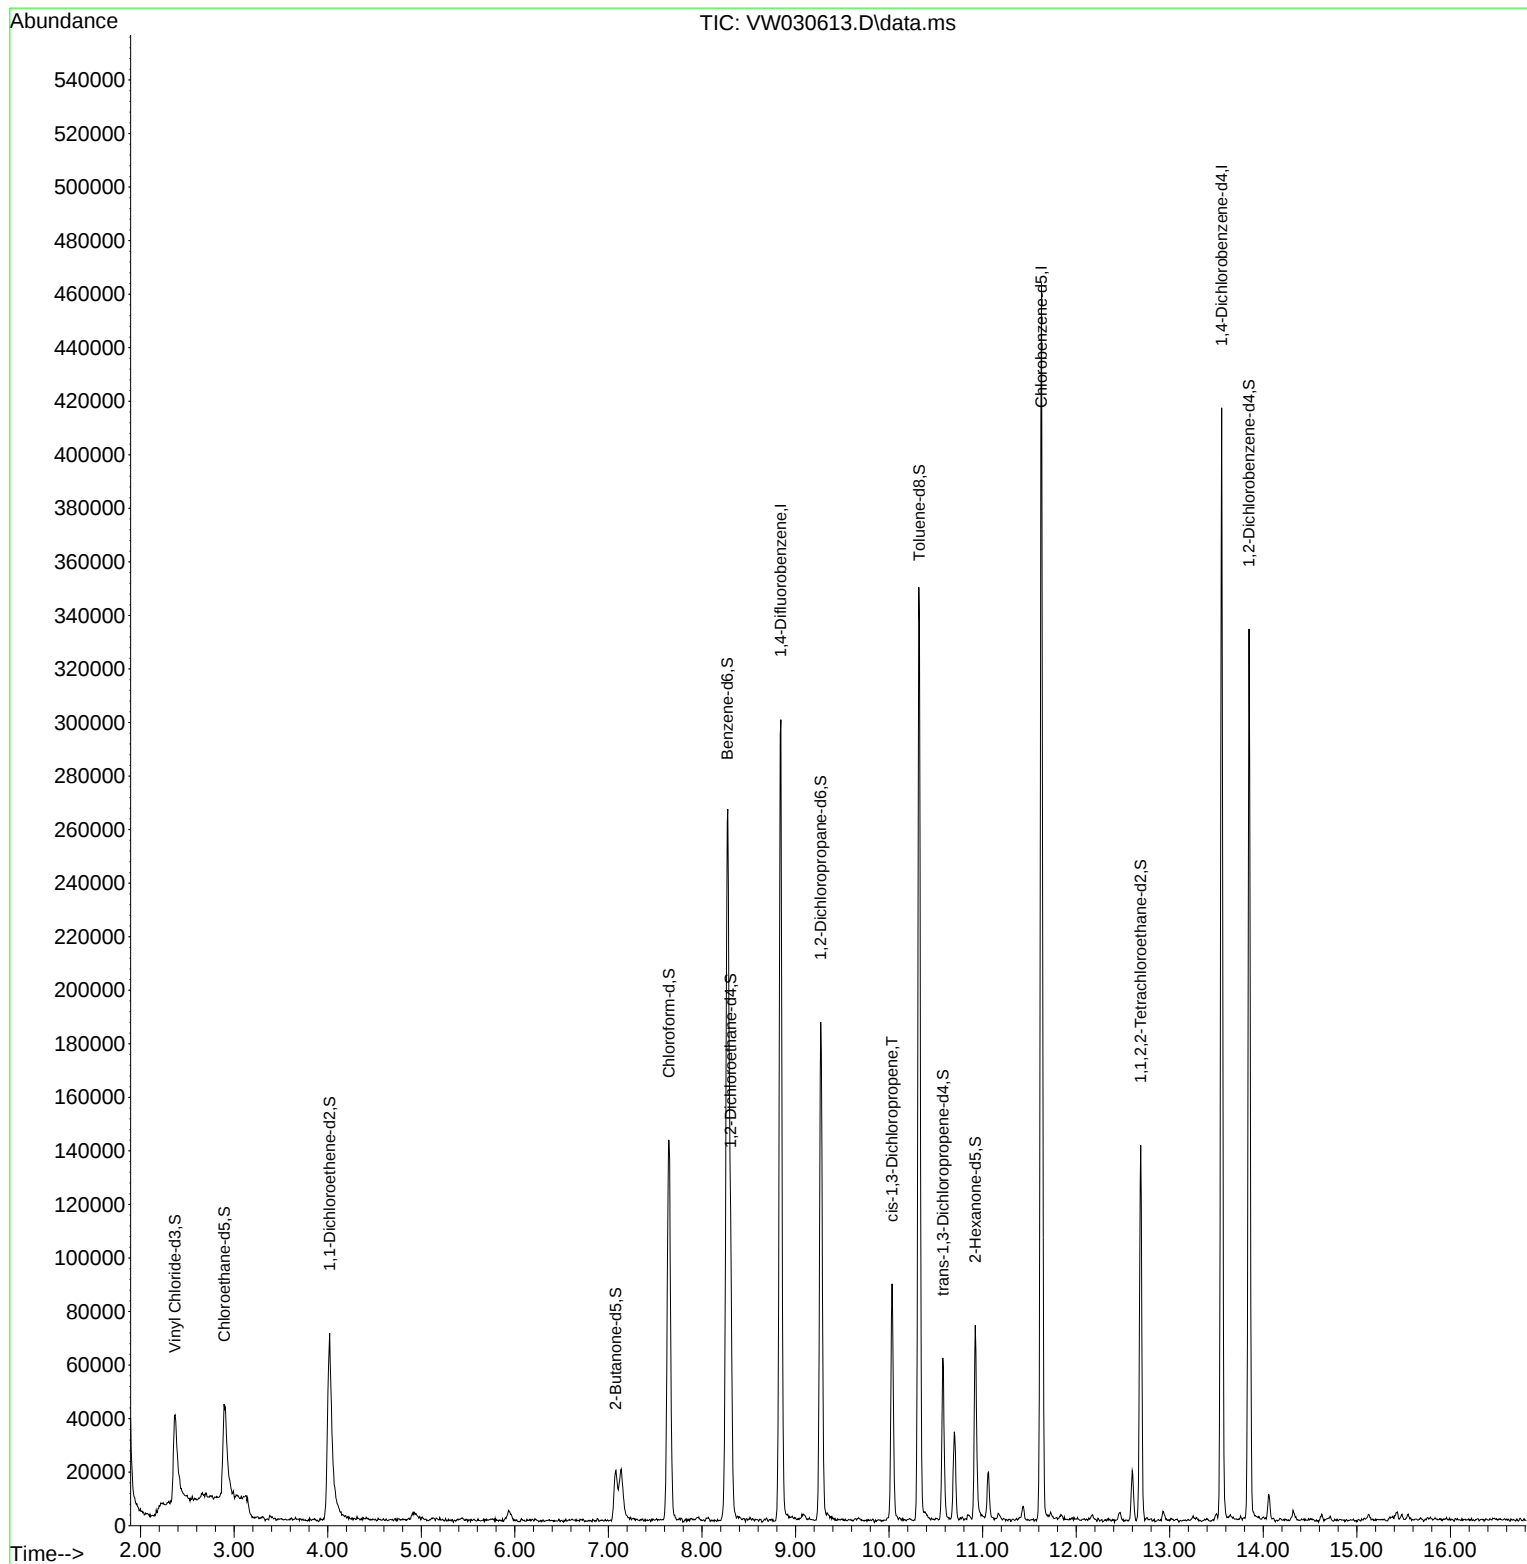

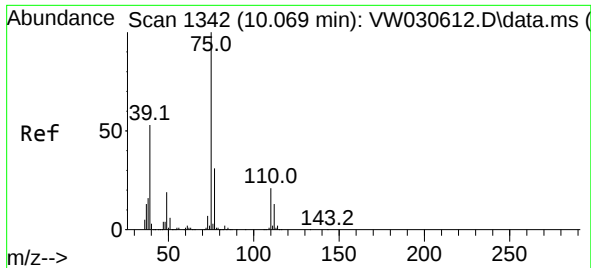

#39
 cis-1,3-Dichloropropene
 Concen: 0.497 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030613.D
 Acq: 16 Oct 2024 15:58

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2839
 Ion Ratio Lower Upper
 75 100
 77 46.5 21.1 39.1#

