

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101624\
 Data File : VW030618.D
 Acq On : 16 Oct 2024 18:00
 Operator : SY/MD
 Sample : P4414-08
 Misc : 4.94g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 17 01:55:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 17 01:53:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	472373	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	383511	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	145518	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	77054	10.378	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	41.520%
7) Chloroethane-d5	2.893	69	79520	14.148	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.600%
11) 1,1-Dichloroethene-d2	4.021	65	30283	9.806	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	39.240%#
21) 2-Butanone-d5	7.081	46	43423	32.497	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.000%
24) Chloroform-d	7.648	84	227429	16.835	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	67.360%
26) 1,2-Dichloroethane-d4	8.502	65	74	0.011	ug/L	0.20
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	341727	15.352	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	61.400%
36) 1,2-Dichloropropane-d6	9.276	67	127403	19.501	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.000%
41) Toluene-d8	10.325	98	264448	13.014	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	52.040%
43) trans-1,3-Dichloroprop...	10.581	79	42945	15.698	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.800%
47) 2-Hexanone-d5	10.922	63	32447	38.560	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96417	20.095	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	85434	17.352	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	69.400%#
Target Compounds						
					Qvalue	
13) Acetone	4.131	43	18878	9.650	ug/L	94
22) 2-Butanone	7.185	43	7816	3.707	ug/L	100
39) cis-1,3-Dichloropropene	10.032	75	3745	0.398	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101624\
Data File : VW030618.D
Acq On : 16 Oct 2024 18:00
Operator : SY/MD
Sample : P4414-08
Misc : 4.94g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 17 01:55:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 17 01:53:12 2024
Response via : Initial Calibration




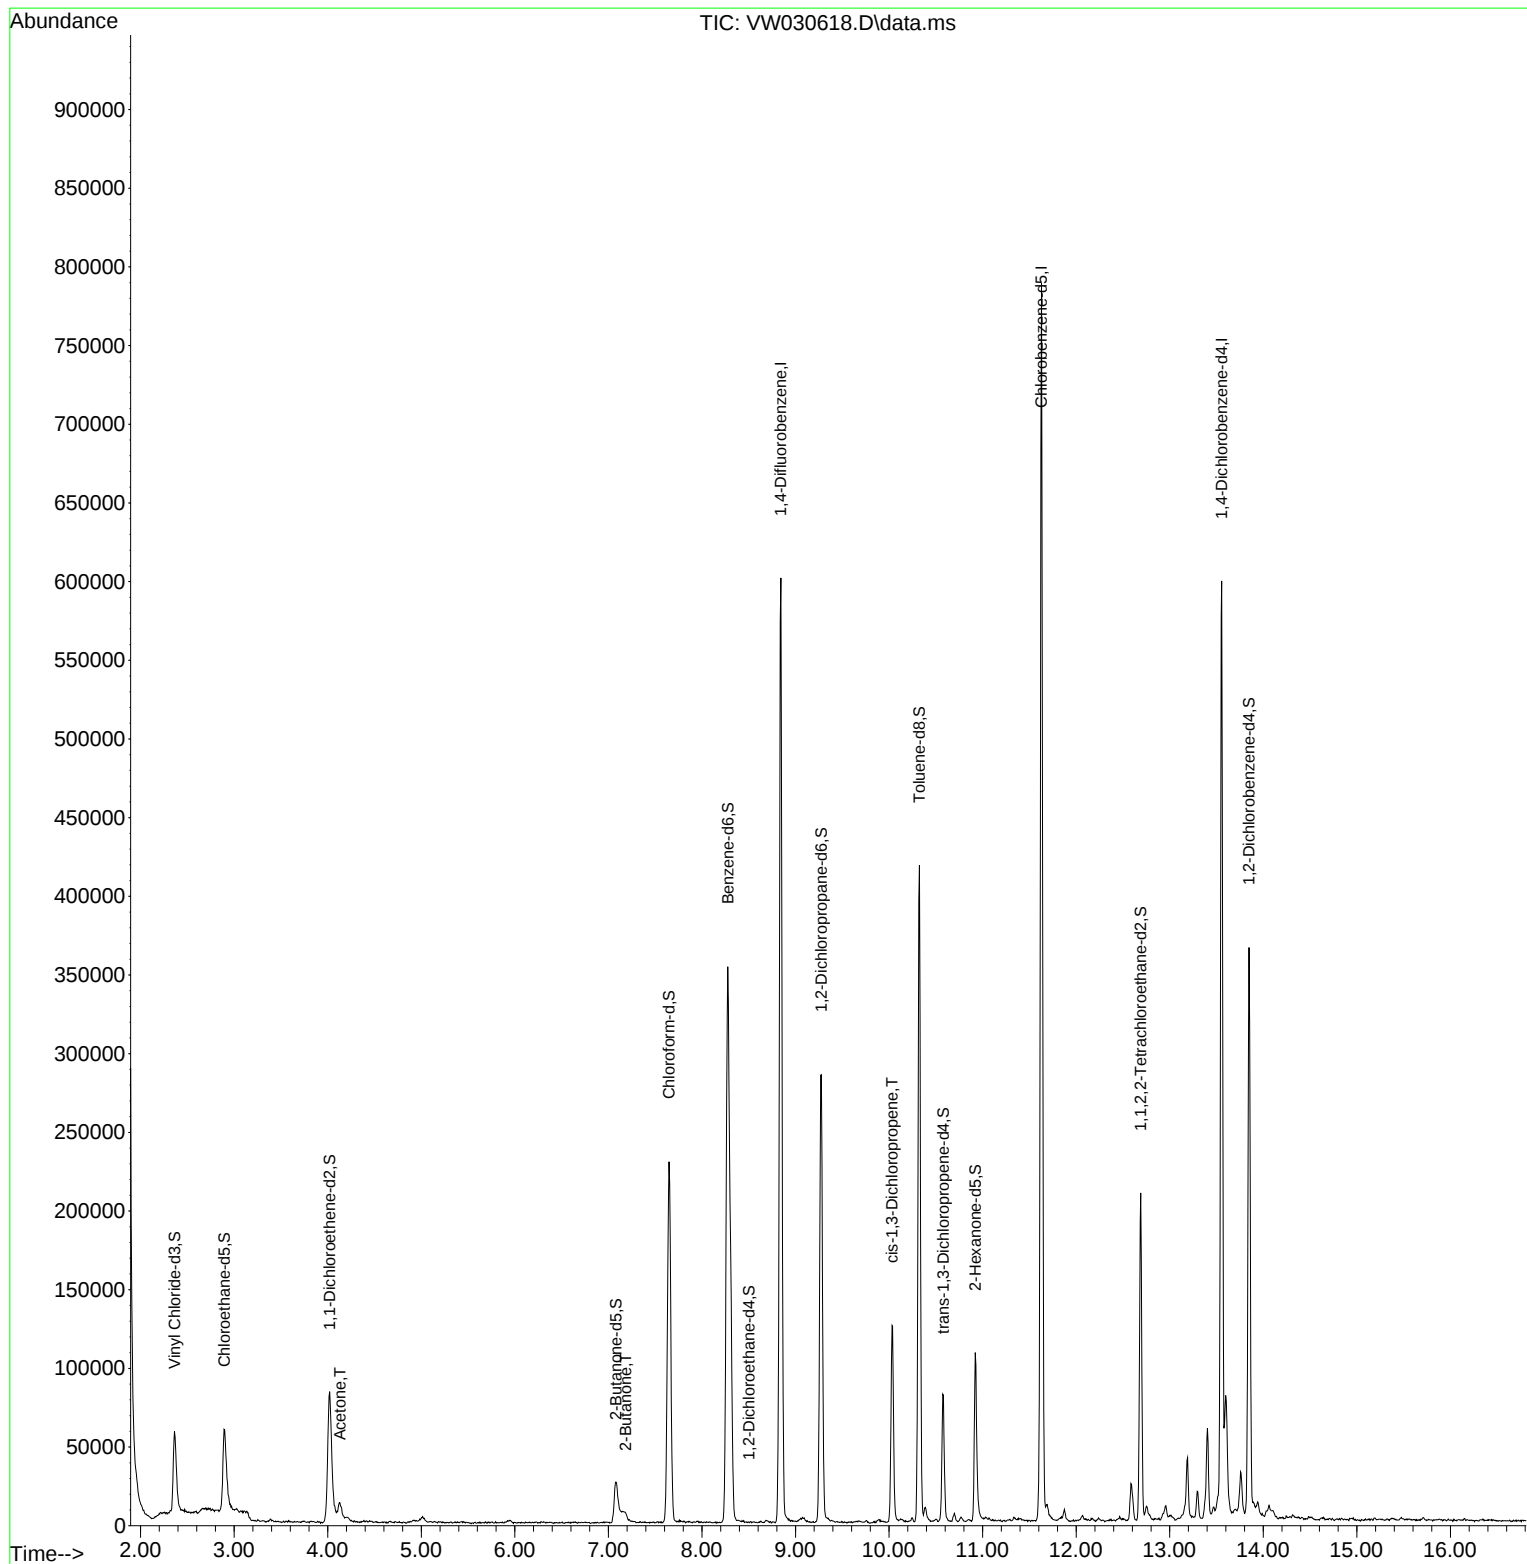


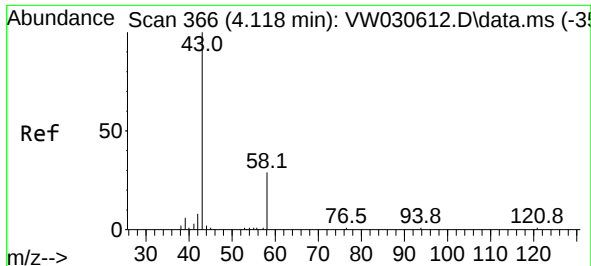

#13
Acetone
Concen: 9.650 ug/L
RT: 4.131 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW030618.D
Acq: 16 Oct 2024 18:00




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 18878
Ion Ratio Lower Upper
43 100
58 32.1 0.0 57.6

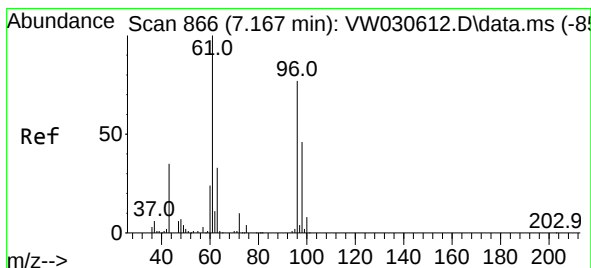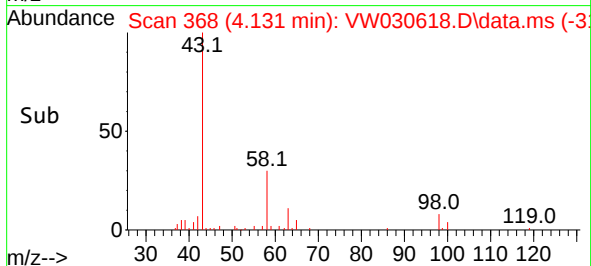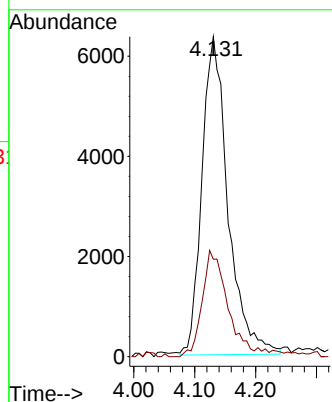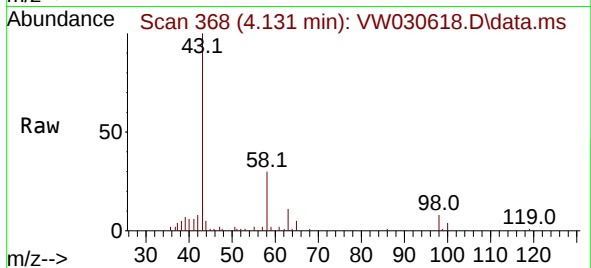

#22
2-Butanone
Concen: 3.707 ug/L
RT: 7.185 min Scan# 869
Delta R.T. 0.018 min
Lab File: VW030618.D
Acq: 16 Oct 2024 18:00


Tgt Ion: 43 Resp: 7816
Ion Ratio Lower Upper
43 100
72 28.7 14.4 43.0

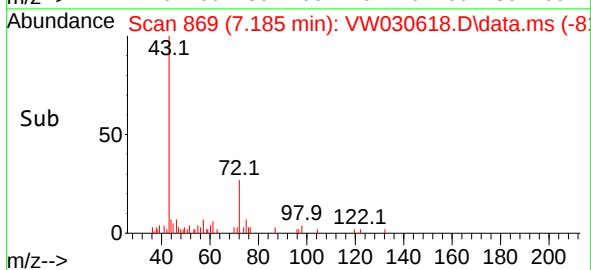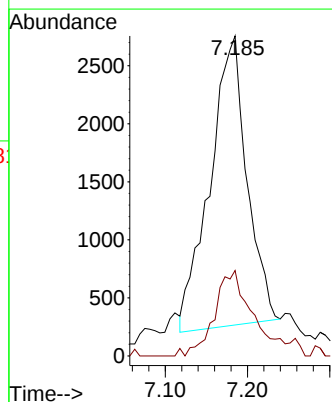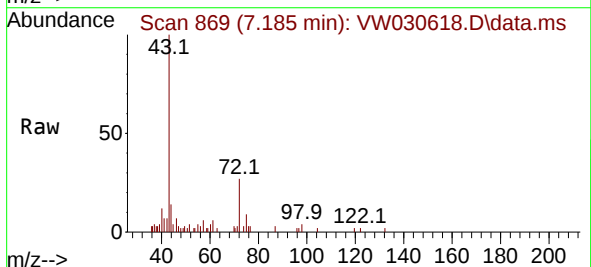

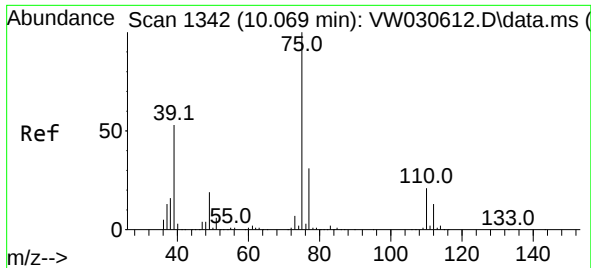

#39
cis-1,3-Dichloropropene
Concen: 0.398 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW030618.D
Acq: 16 Oct 2024 18:00

Instrument :
MSVOA_W
ClientSampleId :

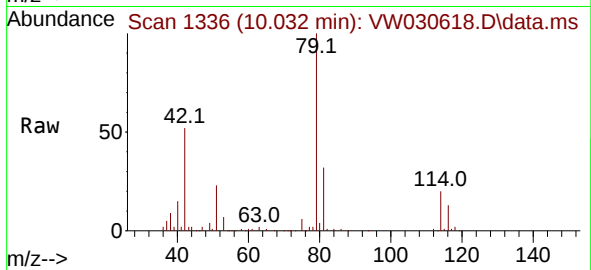

Tgt Ion: 75 Resp: 3745
Ion Ratio Lower Upper
75 100
77 35.4 21.1 39.1

