
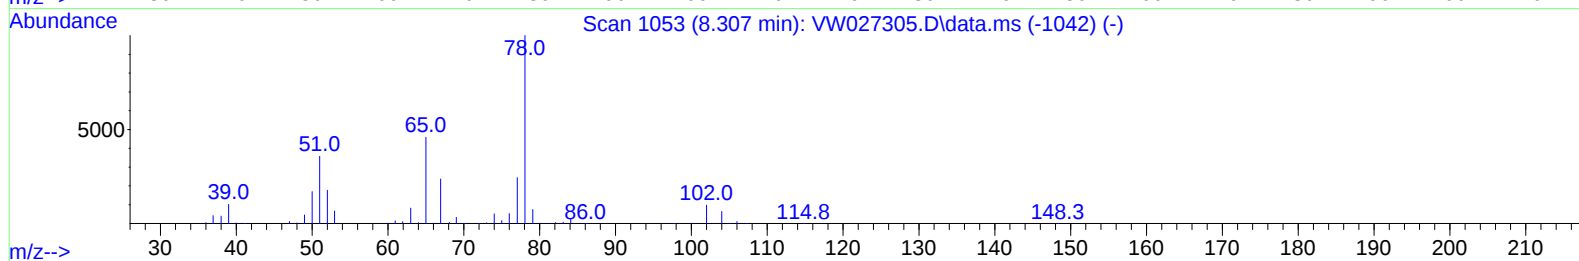
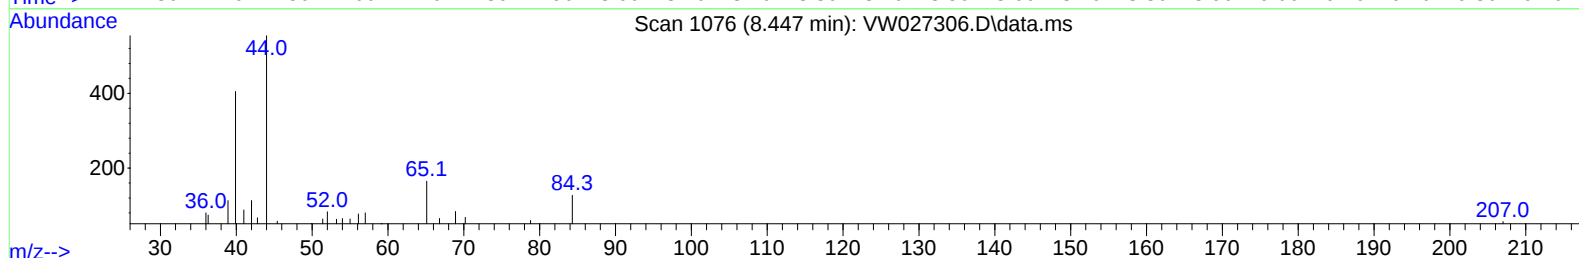


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101723\
Data File : VW027306.D
Acq On : 17 Oct 2023 12:50
Operator : SY/MD
Sample : VW1017SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 05:25:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 16 01:55:11 2023
Response via : Initial Calibration

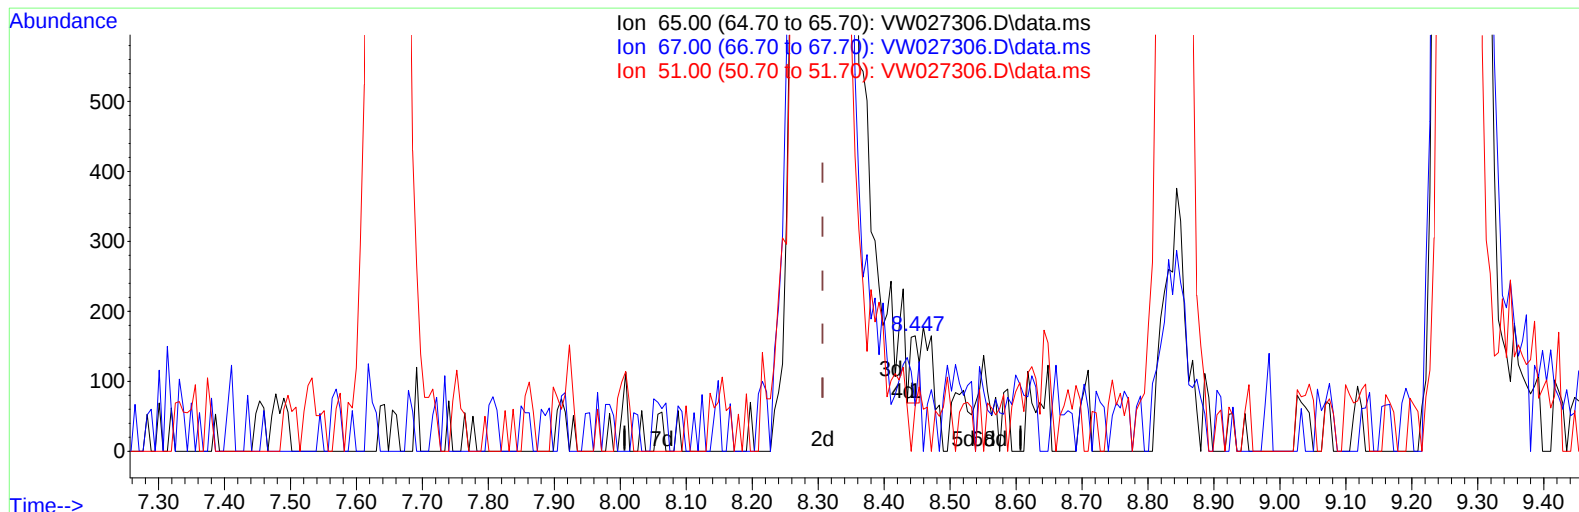

TIC: VW027306.D\data.ms




(26) 1,2-Dichloroethane-d4 (S)

8.447min (+ 0.140) 0.01 ug/L

response	90	
Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	52.22
51.00	99.60	113.33
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101723\
 Data File : VW027306.D
 Acq On : 17 Oct 2023 12:50
 Operator : SY/MD
 Sample : VW1017SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 05:25:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 16 01:55:11 2023
 Response via : Initial Calibration

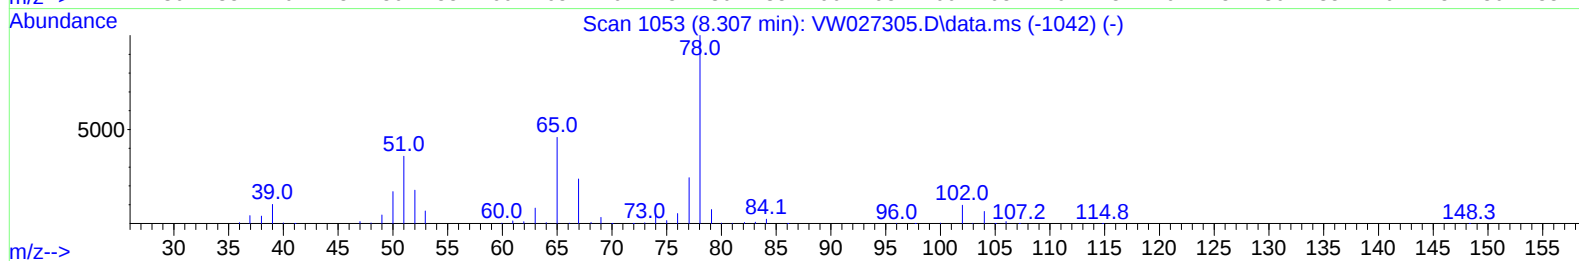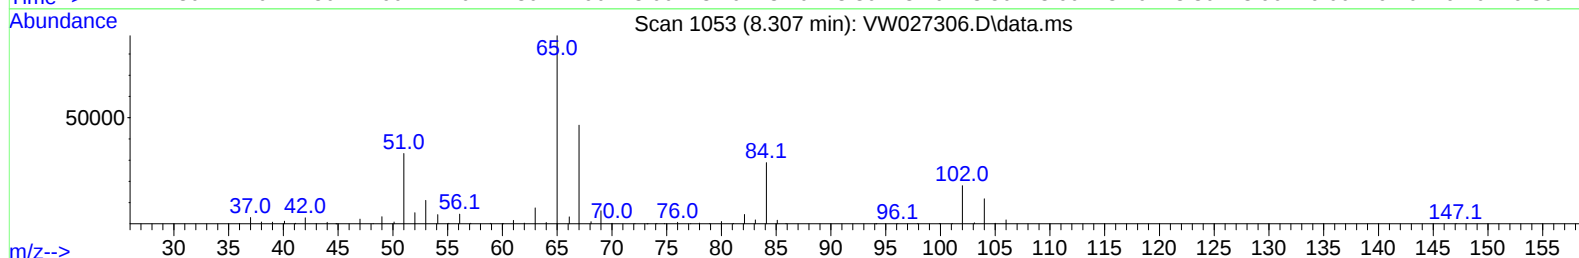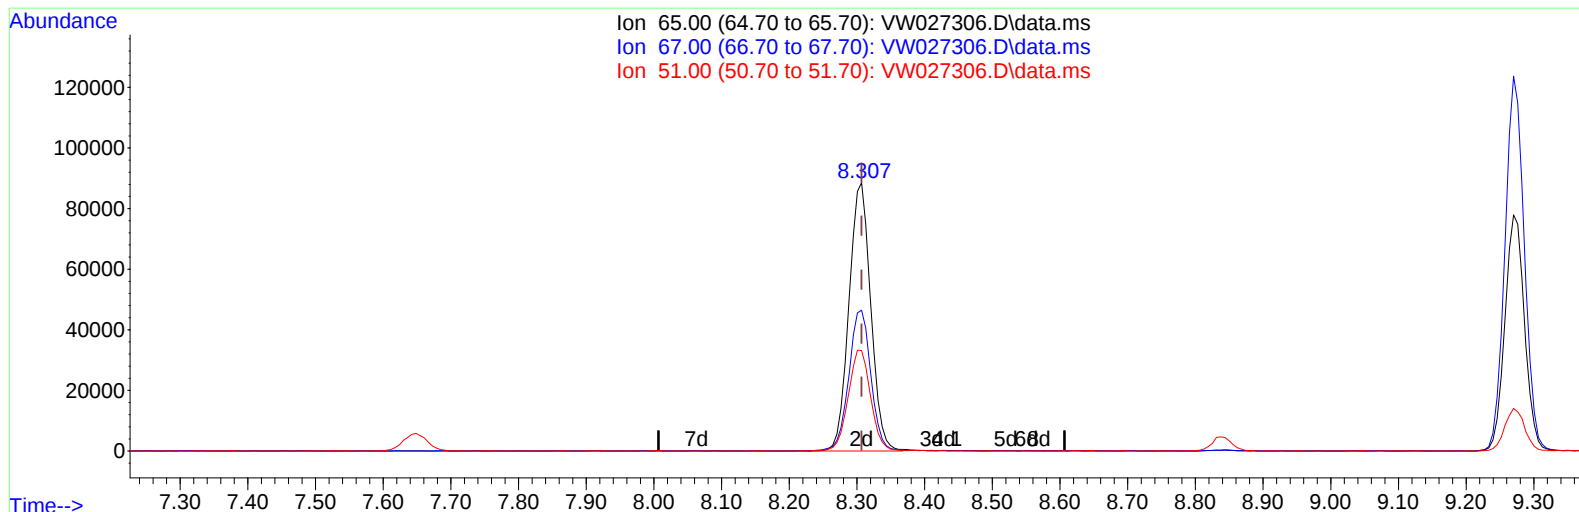

TIC: VW027306.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 25.61 ug/L m****response 197502**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.02#
51.00	99.60	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101723\
 Data File : VW027306.D
 Acq On : 17 Oct 2023 12:50
 Operator : SY/MD
 Sample : VW1017SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 05:25:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Oct 16 01:55:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	481710	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	433464	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	218637	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	198294	26.973	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.880%
7) Chloroethane-d5	2.899	69	151250	28.653	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.600%
11) 1,1-Dichloroethene-d2	4.021	65	97195	26.385	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	105.560%
21) 2-Butanone-d5	7.069	46	102834	42.084	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.160%
24) Chloroform-d	7.648	84	379518	26.434	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.720%
26) 1,2-Dichloroethane-d4	8.307	65	197502m	25.608	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.440%
32) Benzene-d6	8.270	84	822091	28.032	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	112.120%
36) 1,2-Dichloropropane-d6	9.270	67	245975	27.460	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.840%
41) Toluene-d8	10.319	98	724493	27.242	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.960%
43) trans-1,3-Dichloroprop...	10.575	79	101285	24.800	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.200%
47) 2-Hexanone-d5	10.922	63	83332	44.965	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.920%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	162198	24.270	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.080%
66) 1,2-Dichlorobenzene-d4	13.849	152	214748	27.104	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.400%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101723\
Data File : VW027306.D
Acq On : 17 Oct 2023 12:50
Operator : SY/MD
Sample : VW1017SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 05:25:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Oct 16 01:55:11 2023
Response via : Initial Calibration

