

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101823\
 Data File : VW027331.D
 Acq On : 18 Oct 2023 18:07
 Operator : SY/MD
 Sample : 04922-14
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAT3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/19/2023
 Supervised By :Mahesh Dadoda 10/20/2023

Quant Time: Oct 18 22:23:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 18 22:20:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	627752	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	492788	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	170285	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	159020	16.598	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.400%		
7) Chloroethane-d5	2.899	69	126939	18.453	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.800%		
11) 1,1-Dichloroethene-d2	4.021	65	82550	17.196	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	68.800%		
21) 2-Butanone-d5	7.081	46	75372	23.670	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	47.340%		
24) Chloroform-d	7.654	84	352438	18.837	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	75.360%		
26) 1,2-Dichloroethane-d4	8.307	65	189552m	18.860	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	75.440%		
32) Benzene-d6	8.276	84	708505	21.251	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.000%		
36) 1,2-Dichloropropane-d6	9.276	67	226599	22.252	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.000%		
41) Toluene-d8	10.325	98	583044	19.284	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.120%		
43) trans-1,3-Dichloroprop...	10.581	79	77353	16.660	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.640%		
47) 2-Hexanone-d5	10.922	63	62801	29.807	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	59.620%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	144552	19.025	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	76.120%		
66) 1,2-Dichlorobenzene-d4	13.848	152	110776	17.952	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	71.800%#		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	54330	4.728	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101823\
Data File : VW027331.D
Acq On : 18 Oct 2023 18:07
Operator : SY/MD
Sample : 04922-14
Misc : 4.72g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAT3

Quant Time: Oct 18 22:23:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 18 22:20:28 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/19/2023
Supervised By :Mahesh Dadoda 10/20/2023

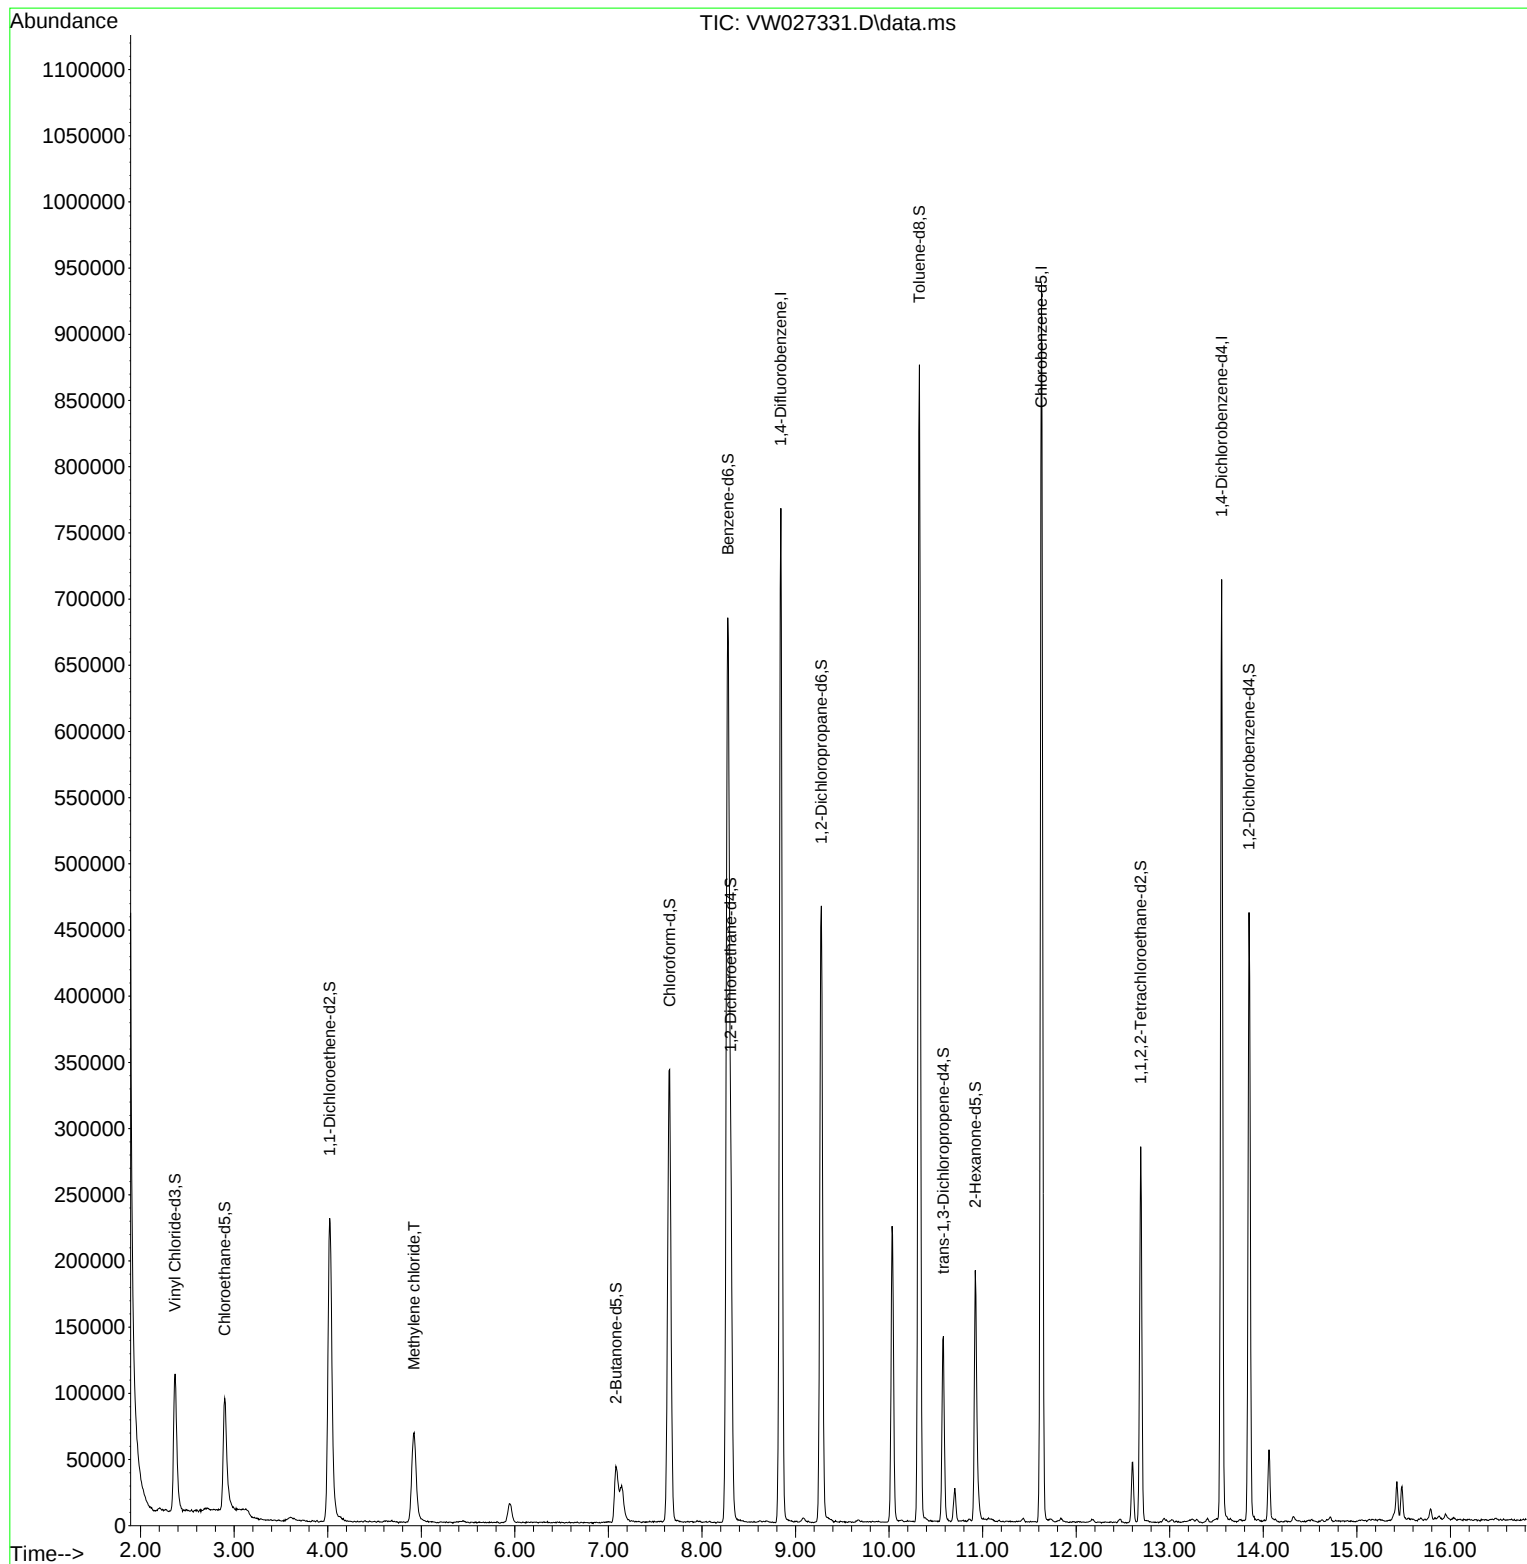

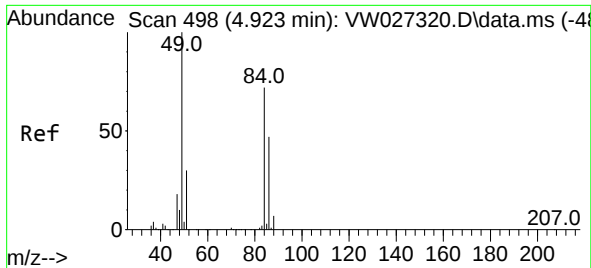

#16
Methylene chloride
Concen: 4.728 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW027331.D
Acq: 18 Oct 2023 18:07

Instrument :
MSVOA_W
ClientSampleId :
EOAT3

Tgt Ion: 84 Resp: 54330
Ion Ratio Lower Upper
84 100
86 62.9 41.3 76.7
49 136.0 92.8 172.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/19/2023
Supervised By :Mahesh Dadoda 10/20/2023

