




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030656.D
Acq On : 18 Oct 2024 11:46
Operator : SY/MD
Sample : P4414-23
Misc : 5.11g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F86

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:25:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

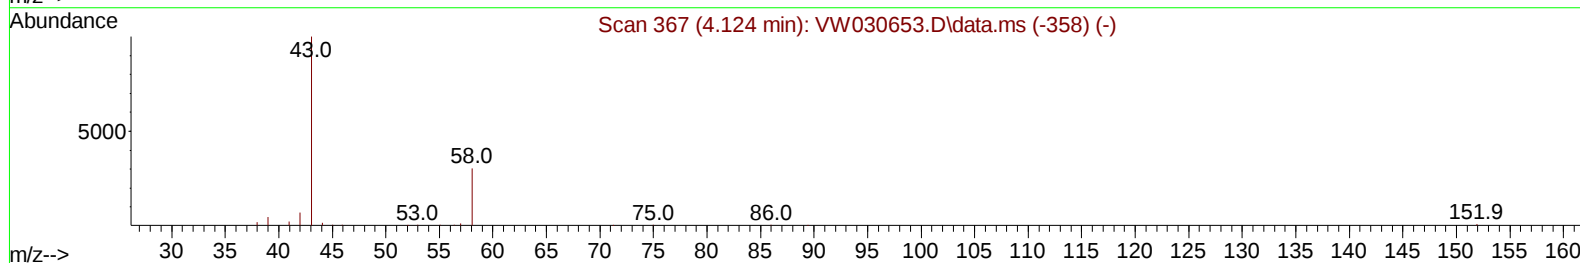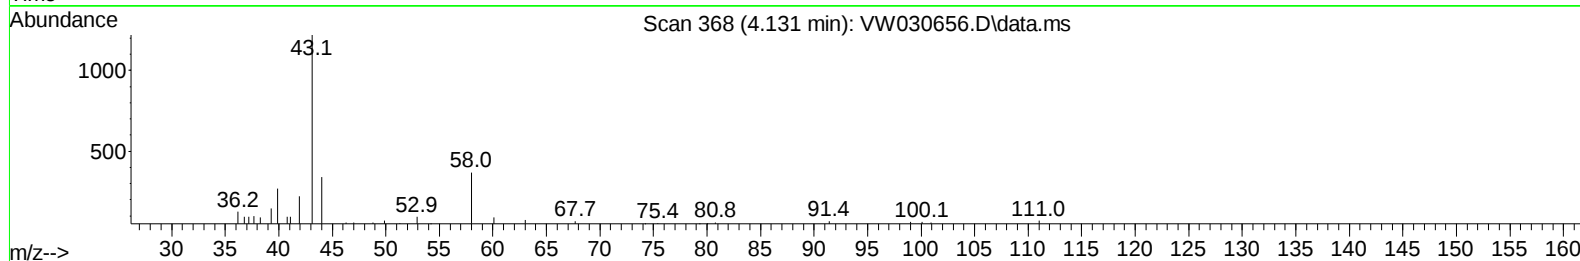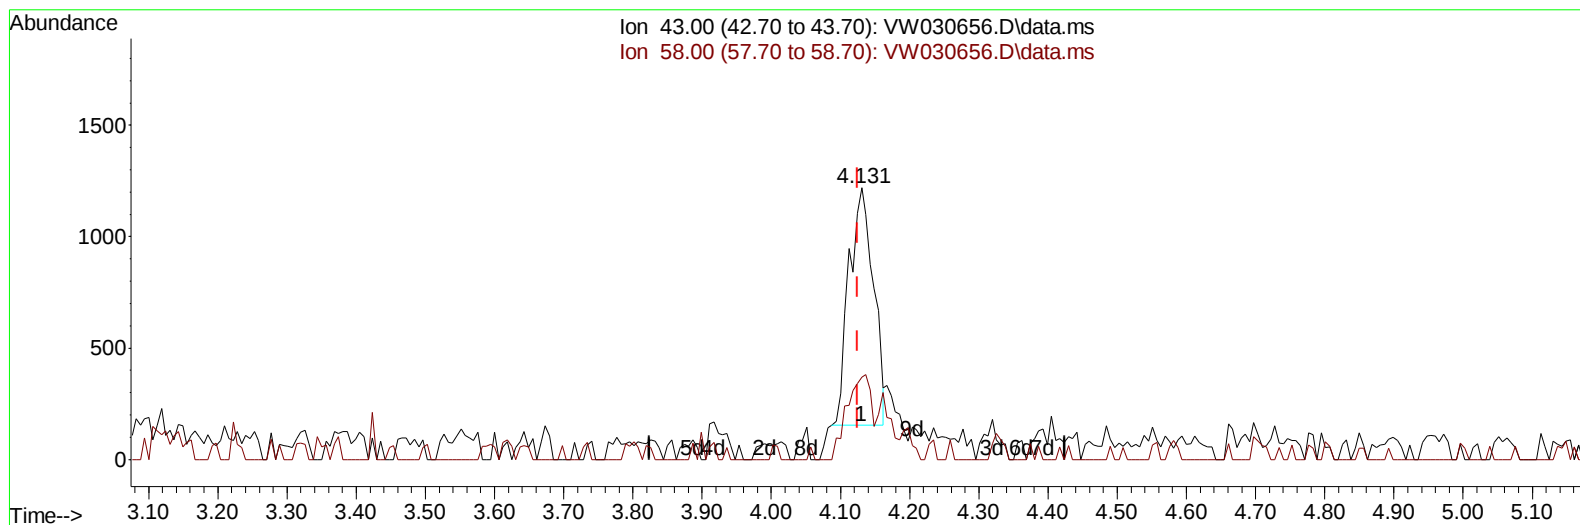

TIC: VW030656.D\data.ms

(13) Acetone (T)

4.131min (+ 0.006) 4.93 ug/L

response 2607

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.80	35.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
 Data File : VW030656.D
 Acq On : 18 Oct 2024 11:46
 Operator : SY/MD
 Sample : P4414-23
 Misc : 5.11g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F86

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:25:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

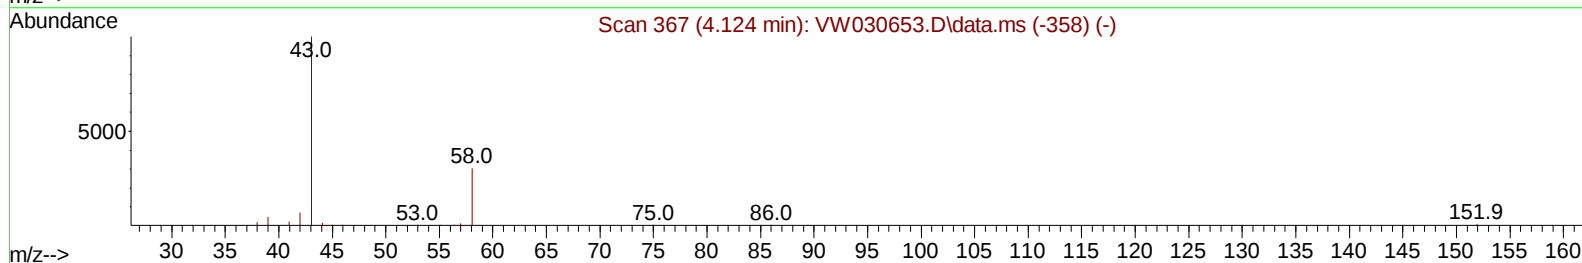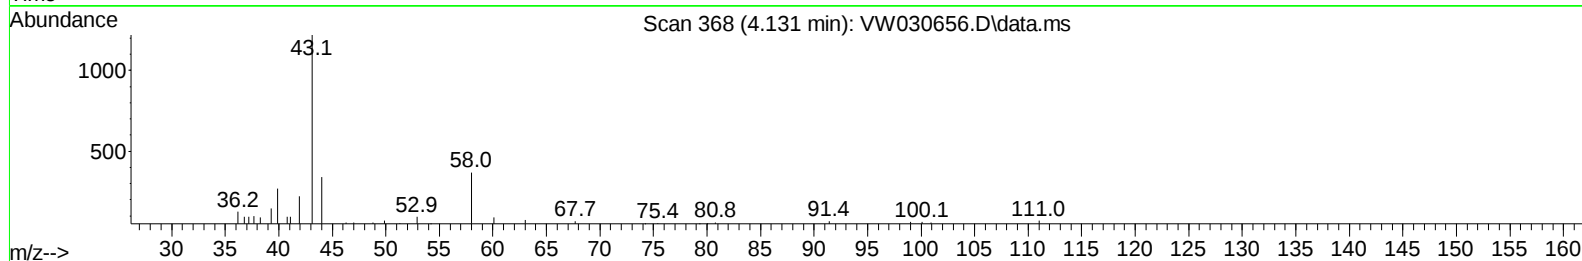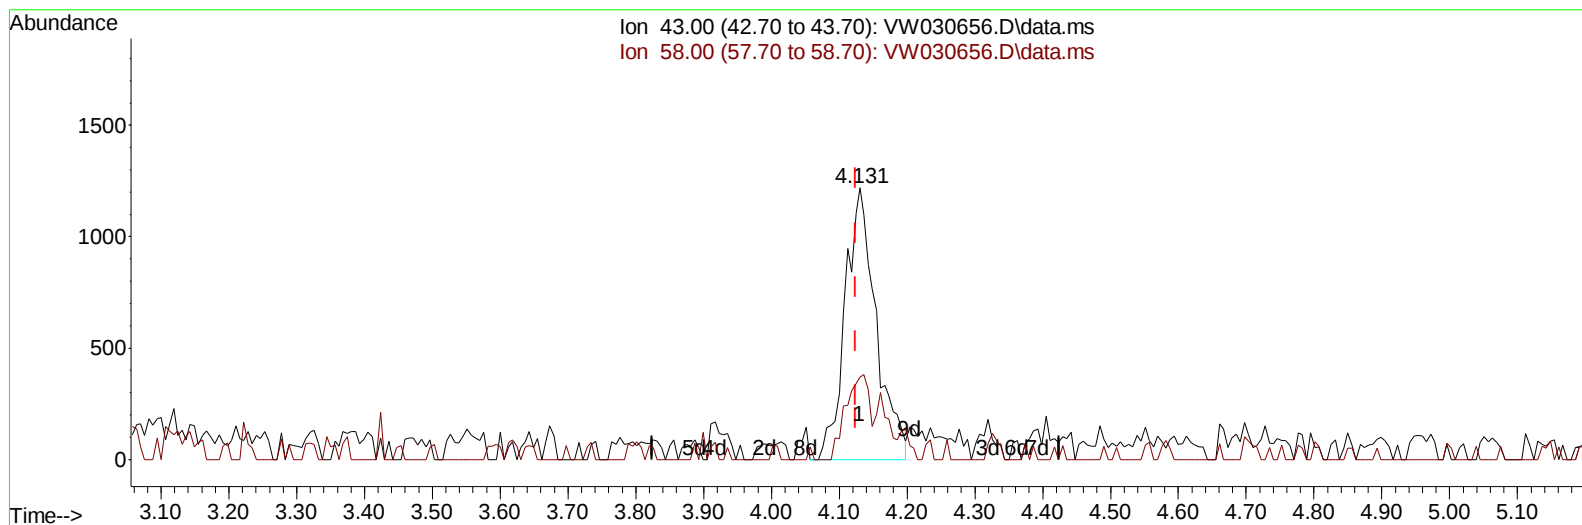

TIC: VW030656.D\data.ms

(13) Acetone (T)

4.131min (+ 0.006) 7.31 ug/L m

response 3866

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.80	23.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101824\
 Data File : VW030656.D
 Acq On : 18 Oct 2024 11:46
 Operator : SY/MD
 Sample : P4414-23
 Misc : 5.11g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F86

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:25:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		127657	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		120797	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		47664	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.356	65		29972	14.937	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.760%		
7) Chloroethane-d5	2.893	69		32673	21.511	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	86.040%		
11) 1,1-Dichloroethene-d2	4.021	65		9839	11.789	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	47.160%		
21) 2-Butanone-d5	7.081	46		19664	54.455	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	108.900%		
24) Chloroform-d	7.648	84		90962	24.916	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	99.680%		
26) 1,2-Dichloroethane-d4	8.307	65		51166	26.952	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	107.800%		
32) Benzene-d6	8.276	84		118712	16.932	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	67.720%		
36) 1,2-Dichloropropane-d6	9.270	67		50104	24.348	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	97.400%		
41) Toluene-d8	10.325	98		74769	11.682	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	46.720%		
43) trans-1,3-Dichloroprop...	10.575	79		15540	18.035	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	72.120%		
47) 2-Hexanone-d5	10.922	63		12944	48.837	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	97.680%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		46689	30.894	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	123.560%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		32204	19.968	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	79.880%		
Target Compounds							Qvalue
13) Acetone	4.131	43		3866m	7.313	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030656.D
Acq On : 18 Oct 2024 11:46
Operator : SY/MD
Sample : P4414-23
Misc : 5.11g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F86

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:25:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

