



Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
 Data File : VW030666.D
 Acq On : 18 Oct 2024 15:53
 Operator : SY/MD
 Sample : P4429-20
 Misc : 4.93g/ 10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F66

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:28:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

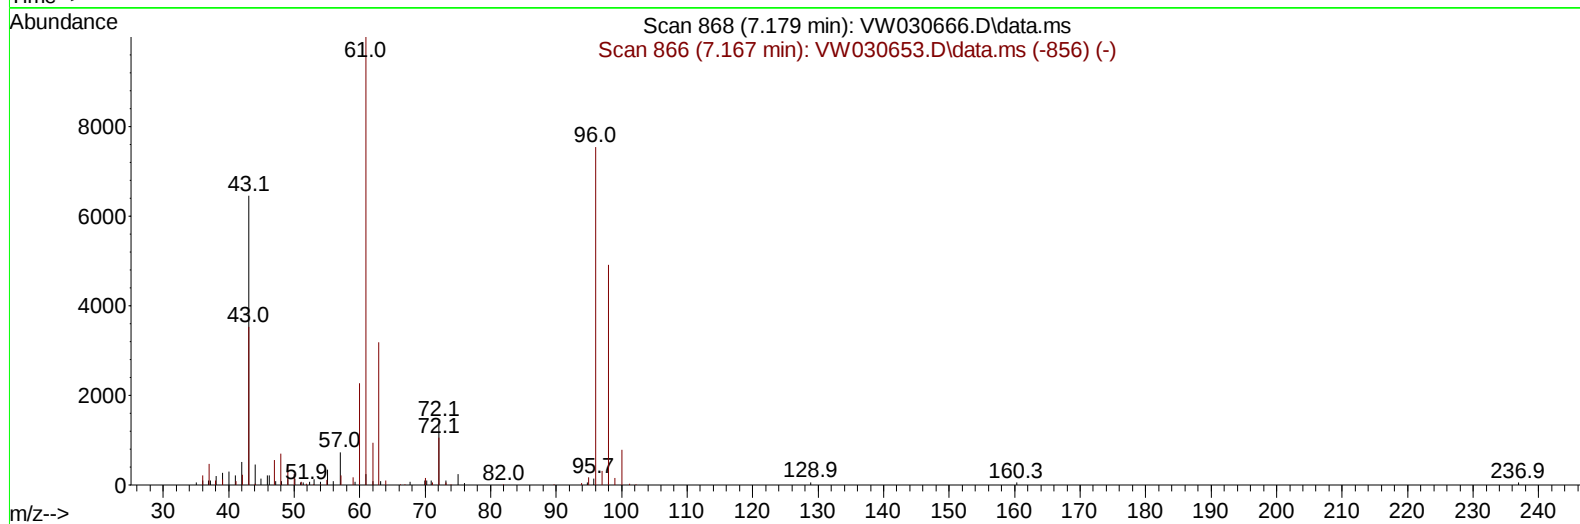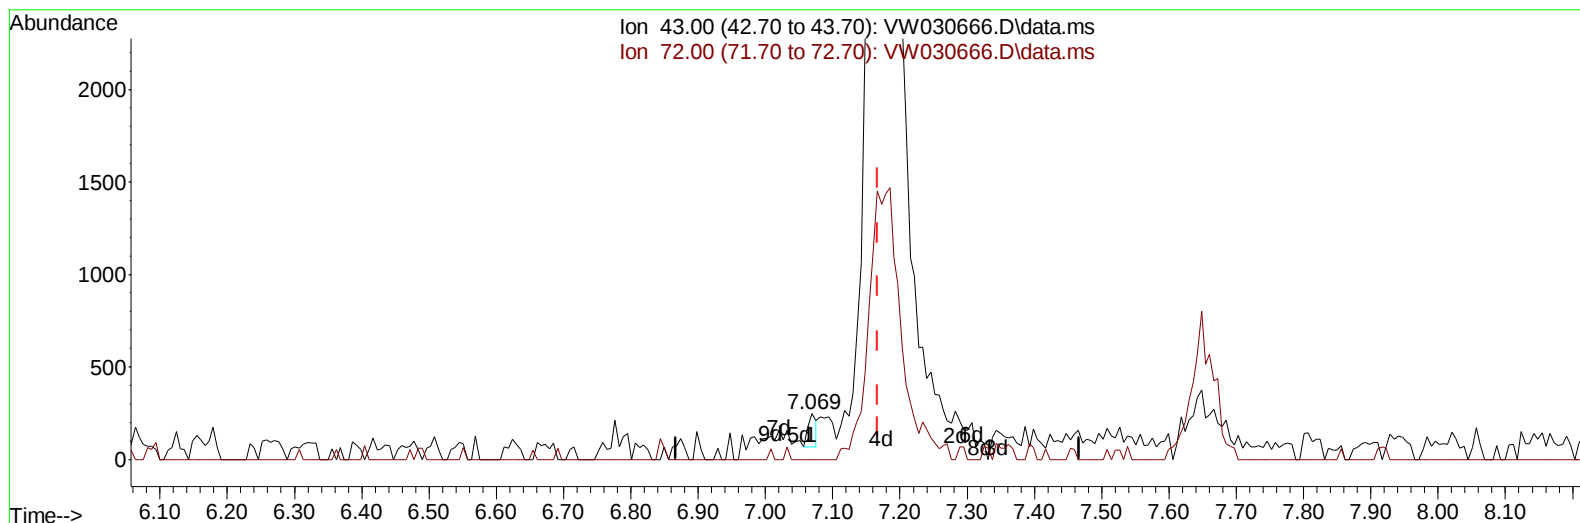

TIC: VW030666.D\data.ms

(22) 2-Butanone (T)

7.069min (-0.098) 0.09 ug/L

response 155

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.70	41.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030666.D
Acq On : 18 Oct 2024 15:53
Operator : SY/MD
Sample : P4429-20
Misc : 4.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F66

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:28:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

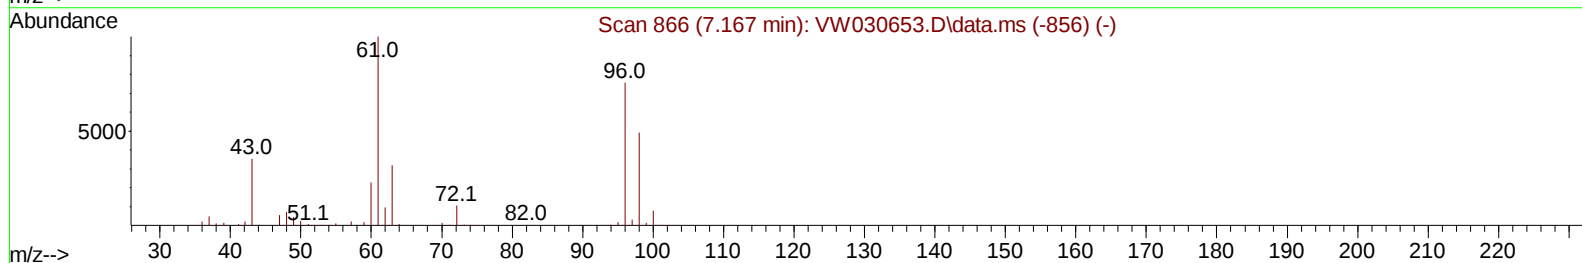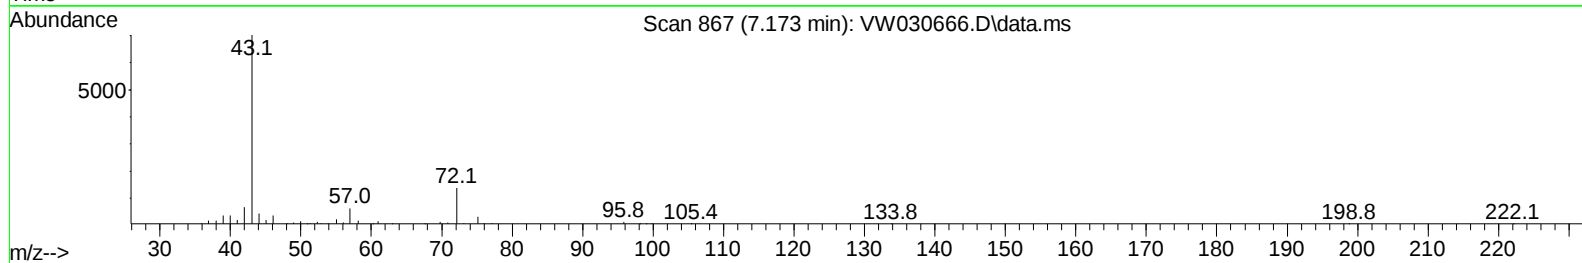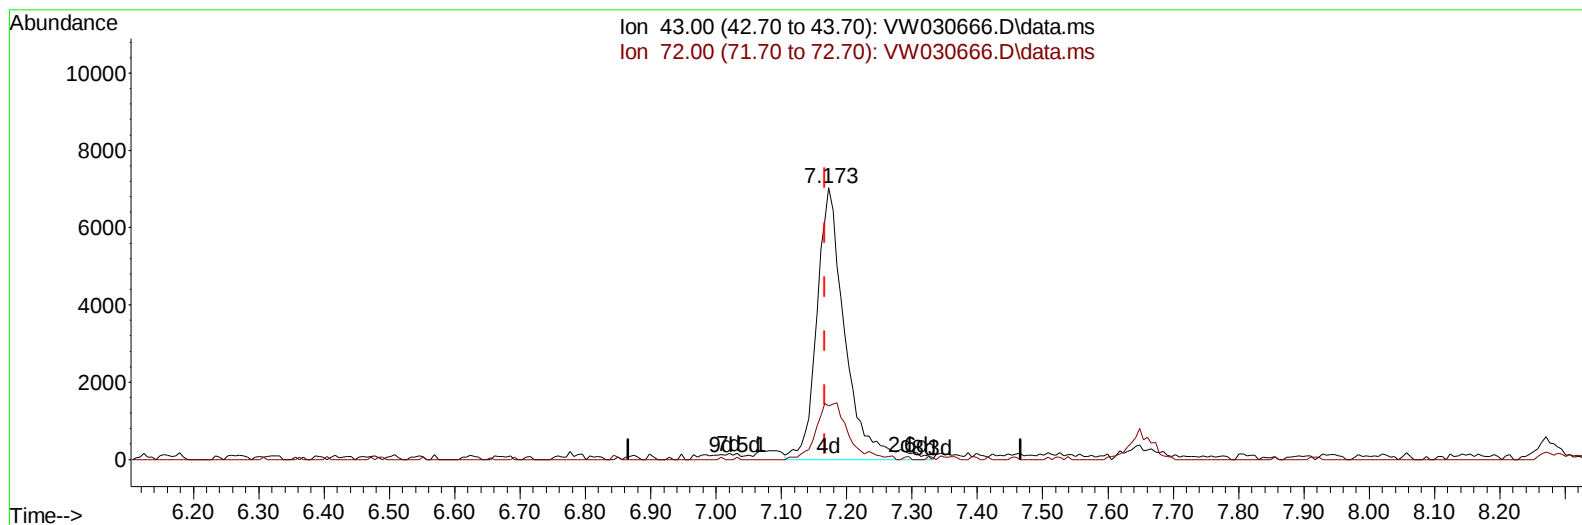

TIC: VW030666.D\data.ms

(22) 2-Butanone (T)

7.173min (+ 0.006) 12.18 ug/L m

response 21019

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.70	0.30#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030666.D
Acq On : 18 Oct 2024 15:53
Operator : SY/MD
Sample : P4429-20
Misc : 4.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F66

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:28:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

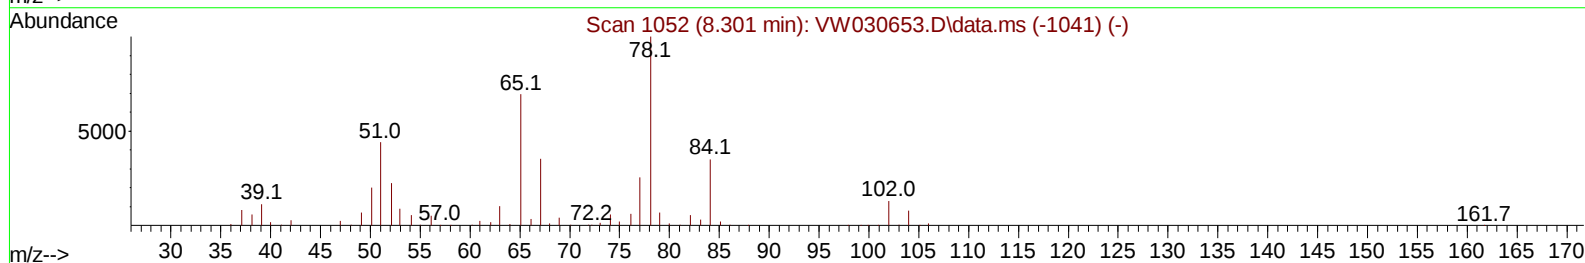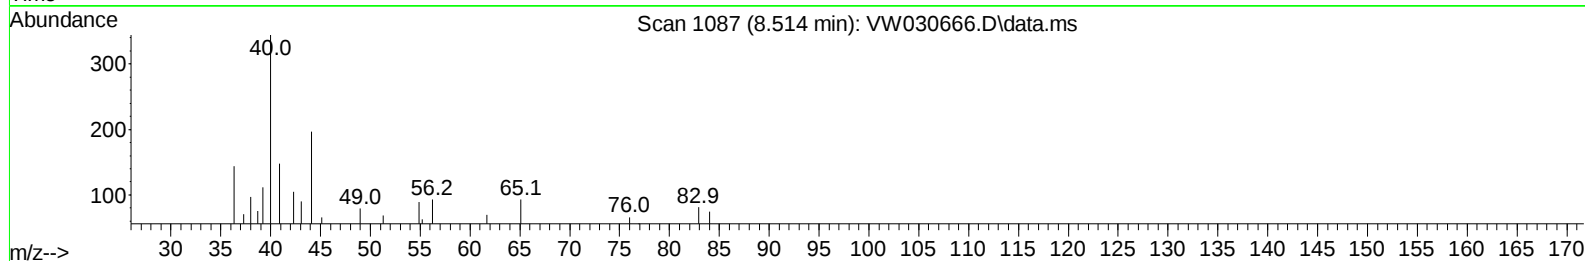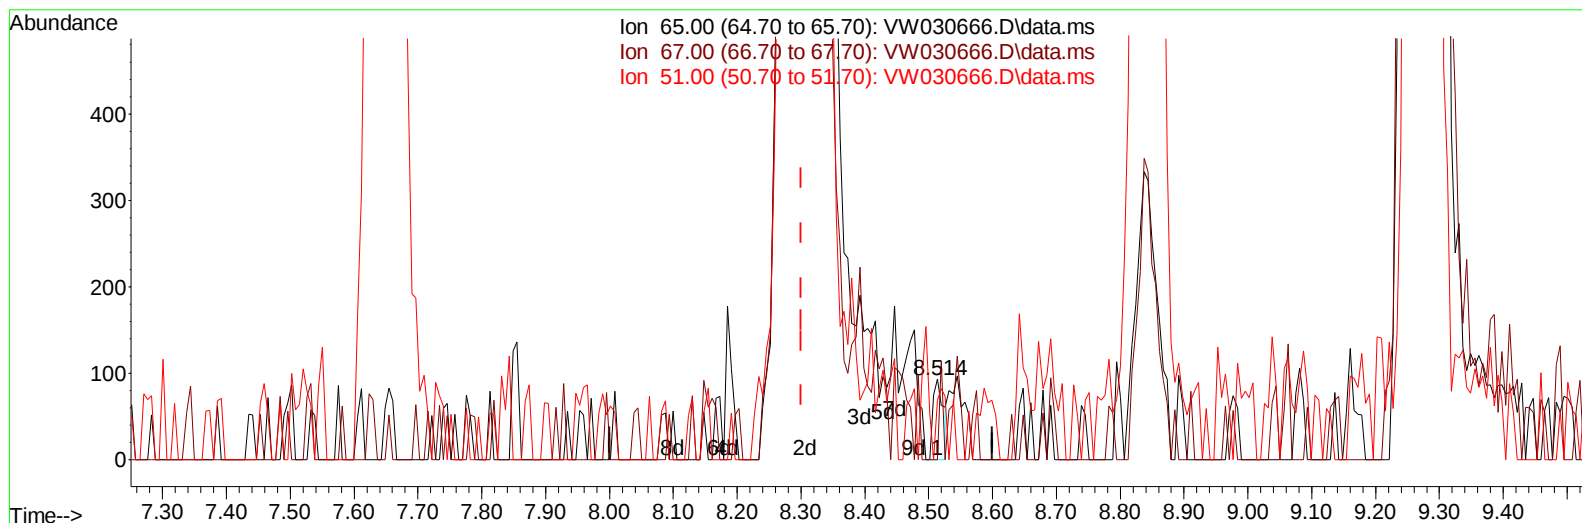

TIC: VW030666.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.514min (+ 0.213) 0.02 ug/L

response 107

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	39.25
51.00	109.40	76.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030666.D
Acq On : 18 Oct 2024 15:53
Operator : SY/MD
Sample : P4429-20
Misc : 4.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F66

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:28:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

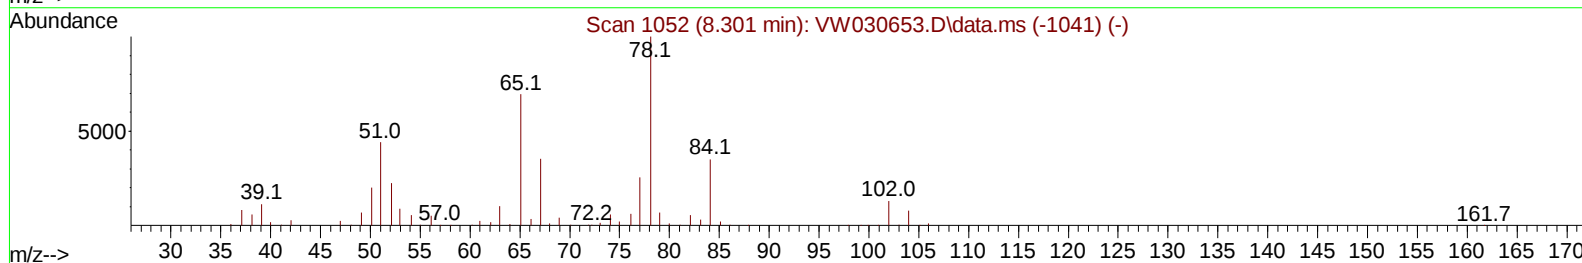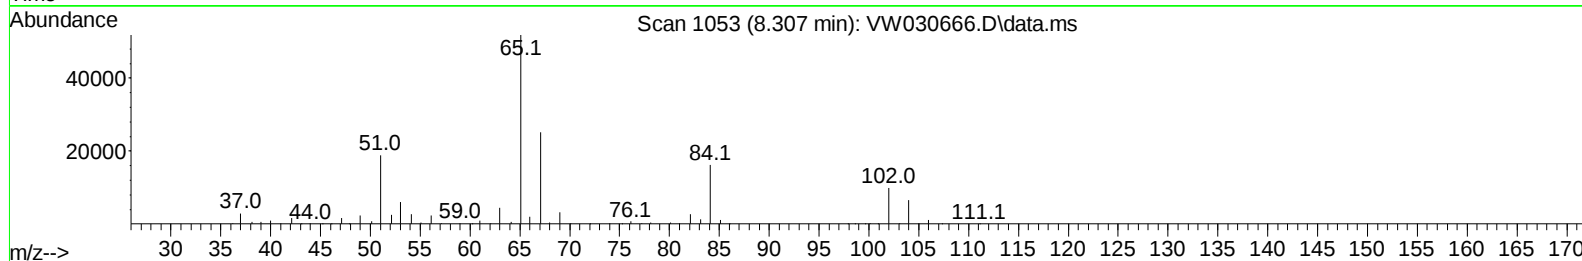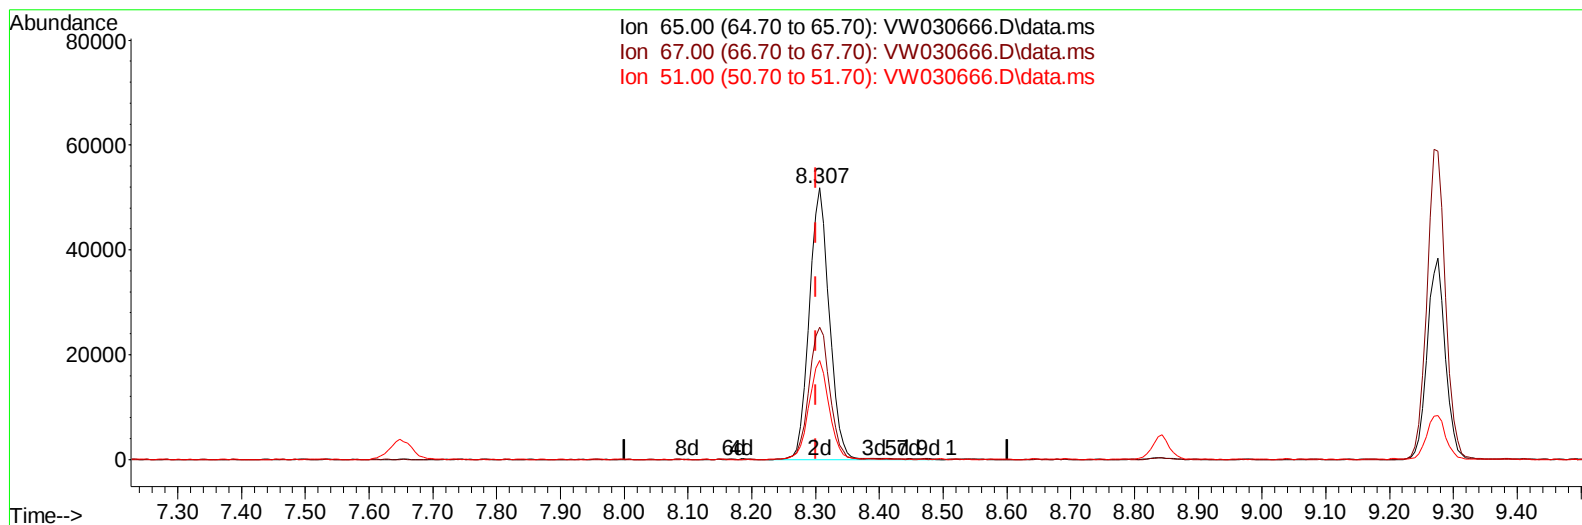

TIC: VW030666.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 19.70 ug/L m

response 113279

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.04#
51.00	109.40	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101824\
 Data File : VW030666.D
 Acq On : 18 Oct 2024 15:53
 Operator : SY/MD
 Sample : P4429-20
 Misc : 4.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F66

Manual IntegrationsAPPROVED

Quant Time: Oct 19 00:28:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	386644	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	322587	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	115441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74627	12.279	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	49.120%		
7) Chloroethane-d5	2.899	69	74180	16.125	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	64.480%		
11) 1,1-Dichloroethene-d2	4.021	65	29911	11.833	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	47.320%		
21) 2-Butanone-d5	7.075	46	46978	42.953	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	85.900%		
24) Chloroform-d	7.648	84	212057	19.178	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	76.720%		
26) 1,2-Dichloroethane-d4	8.307	65	113279m	19.701	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	78.800%		
32) Benzene-d6	8.276	84	327984	17.518	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	70.080%		
36) 1,2-Dichloropropane-d6	9.270	67	119394	21.726	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	86.920%		
41) Toluene-d8	10.325	98	248339	14.530	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	58.120%		
43) trans-1,3-Dichloroprop...	10.575	79	40180	17.461	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	69.840%		
47) 2-Hexanone-d5	10.922	63	33827	47.792	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	95.580%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	87803	21.756	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	87.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152	75883	19.427	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	77.720%		
Target Compounds						
						Qvalue
13) Acetone	4.118	43	45615	28.488	ug/L	94
22) 2-Butanone	7.173	43	21019m	12.178	ug/L	
42) Toluene	10.386	91	32068	1.432	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030666.D
Acq On : 18 Oct 2024 15:53
Operator : SY/MD
Sample : P4429-20
Misc : 4.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F66

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

Quant Time: Oct 19 00:28:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

