

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
 Data File : VW030667.D
 Acq On : 18 Oct 2024 16:17
 Operator : SY/MD
 Sample : P4429-21
 Misc : 5.02g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F67

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

Quant Time: Oct 19 00:28:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	455923	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	370652	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	136602	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74168	10.349	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	41.400%		
7) Chloroethane-d5	2.899	69	78684	14.505	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.000%		
11) 1,1-Dichloroethene-d2	4.021	65	29273	9.821	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	39.280%#		
21) 2-Butanone-d5	7.075	46	50860	39.436	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.880%		
24) Chloroform-d	7.654	84	222734	17.083	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	68.320%		
26) 1,2-Dichloroethane-d4	8.307	65	114114m	16.831	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	67.320%#		
32) Benzene-d6	8.270	84	332430	15.453	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	61.800%		
36) 1,2-Dichloropropane-d6	9.276	67	123522	19.563	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	78.240%		
41) Toluene-d8	10.318	98	252679	12.866	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	51.480%		
43) trans-1,3-Dichloroprop...	10.574	79	41058	15.529	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	62.120%		
47) 2-Hexanone-d5	10.922	63	37399	45.987	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.980%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	92759	20.004	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.000%		
66) 1,2-Dichlorobenzene-d4	13.848	152	80078	17.325	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	69.320%#		
Target Compounds					Qvalue	
13) Acetone	4.124	43	42099	22.297	ug/L	98
22) 2-Butanone	7.167	43	16821	8.265	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030667.D
Acq On : 18 Oct 2024 16:17
Operator : SY/MD
Sample : P4429-21
Misc : 5.02g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4F67

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024


Quant Time: Oct 19 00:28:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

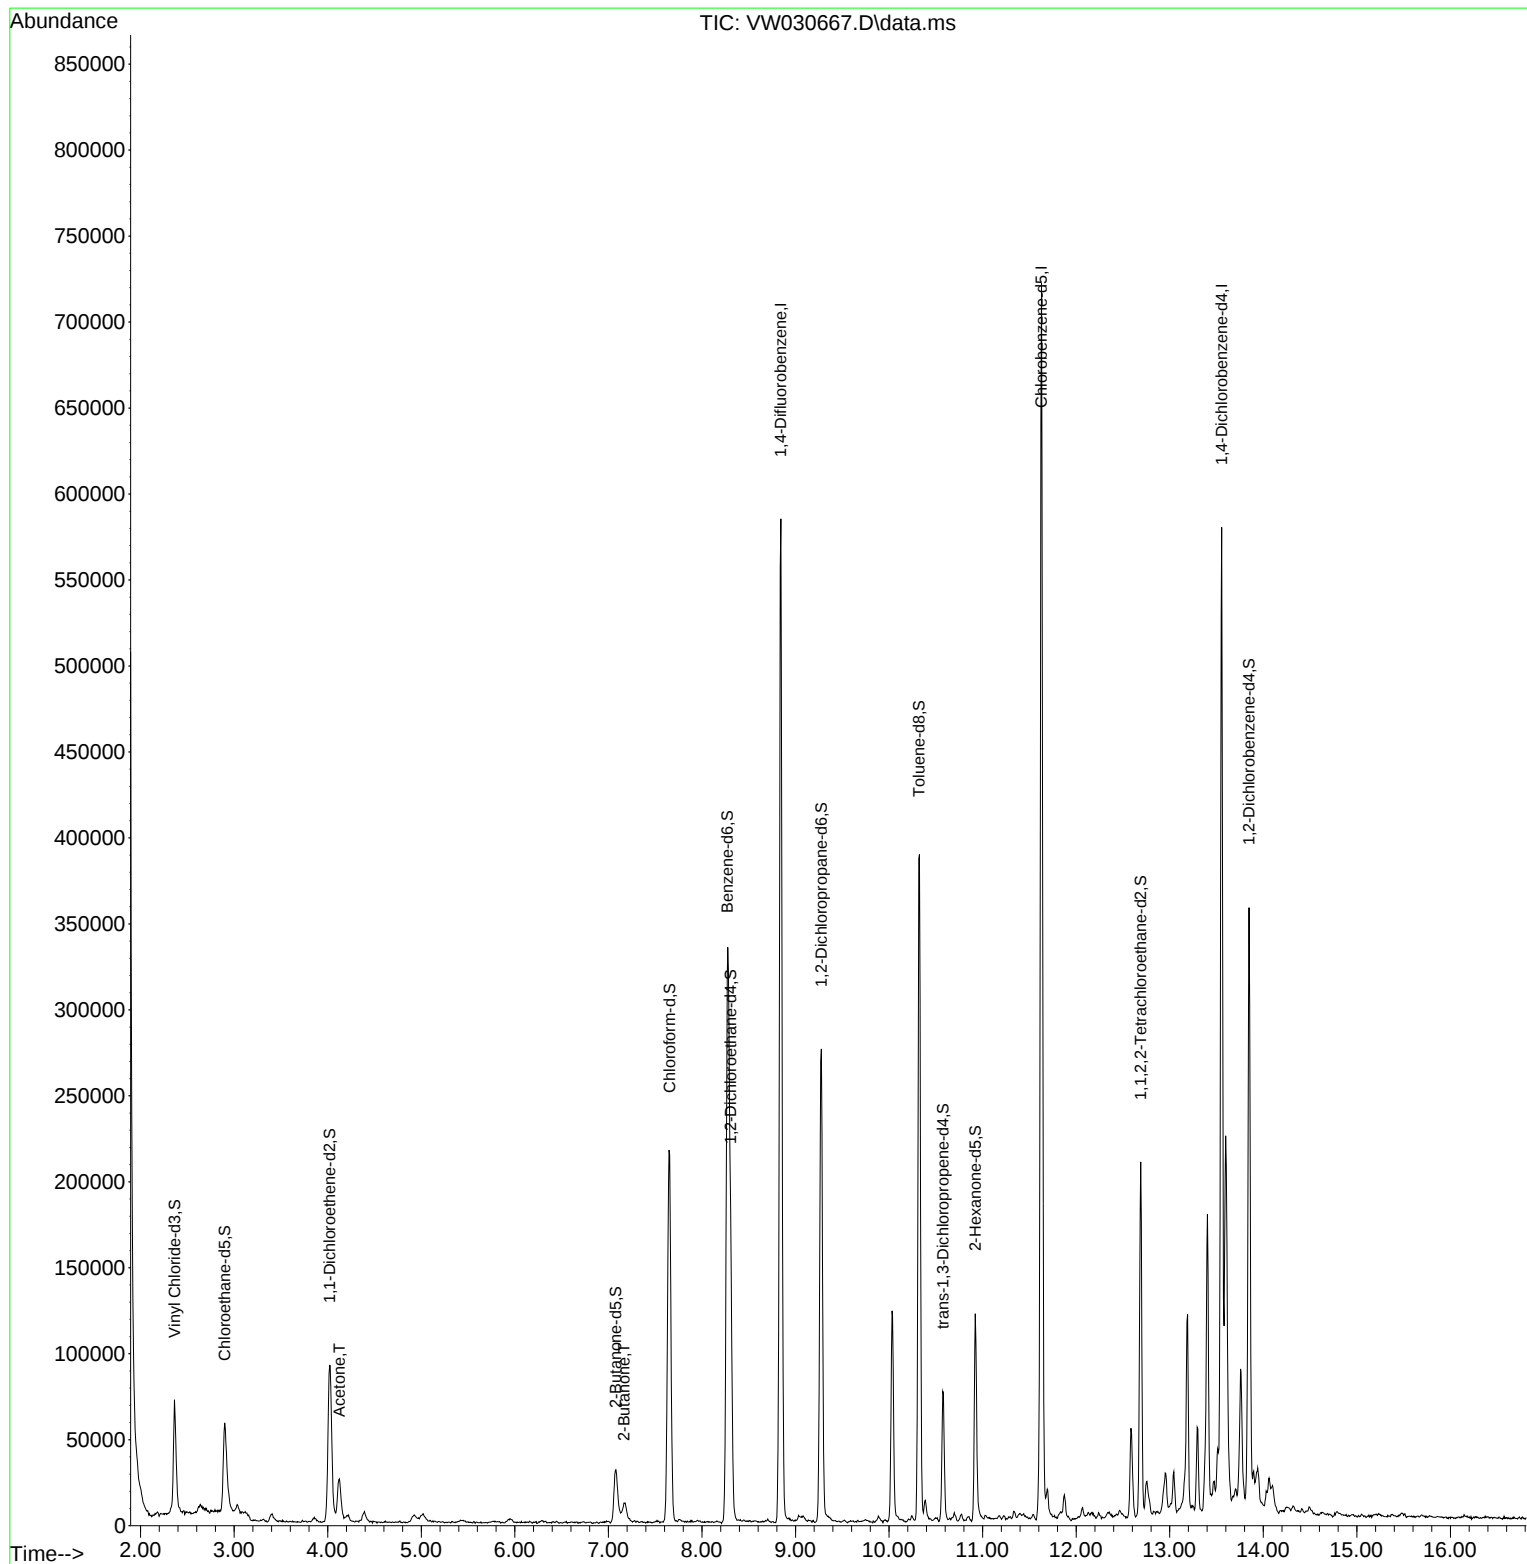

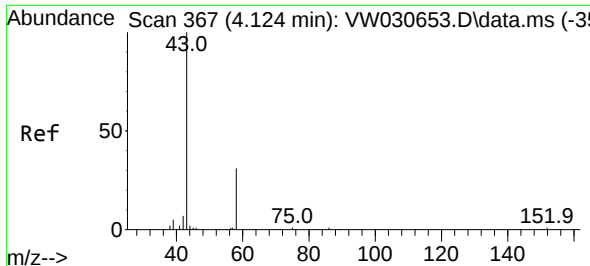

#13
Acetone
Concen: 22.297 ug/L
RT: 4.124 min Scan# 367
Delta R.T. -0.000 min
Lab File: VW030667.D
Acq: 18 Oct 2024 16:17




Instrument :
MSVOA_W
ClientSampleId :
A4F67

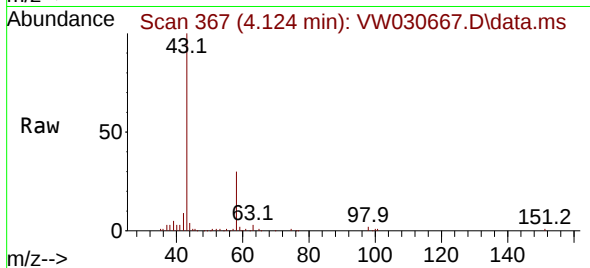

Tgt Ion: 43 Resp: 42099
Ion Ratio Lower Upper
43 100
58 29.8 0.0 57.6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

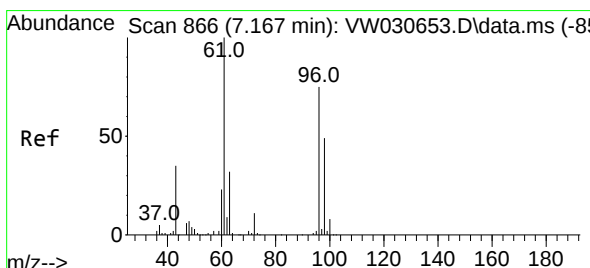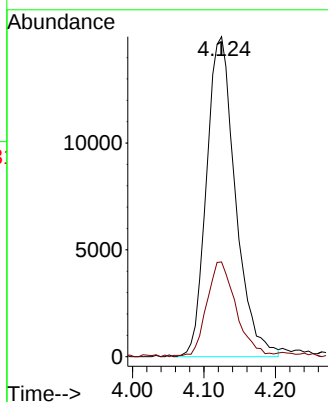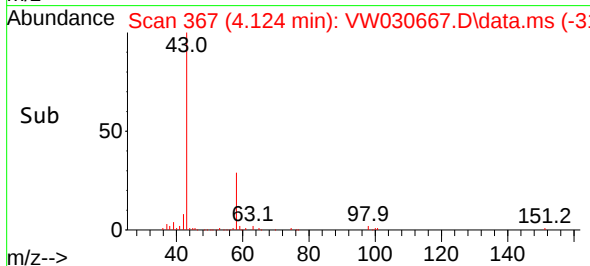

#22
2-Butanone
Concen: 8.265 ug/L
RT: 7.167 min Scan# 866
Delta R.T. -0.000 min
Lab File: VW030667.D
Acq: 18 Oct 2024 16:17

Tgt Ion: 43 Resp: 16821
Ion Ratio Lower Upper
43 100
72 25.3 14.4 43.0

