

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
 Data File : VW030669.D
 Acq On : 18 Oct 2024 17:05
 Operator : SY/MD
 Sample : P4414-21RE
 Misc : 5.79g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F82RE

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
 Supervised By :Semsettin Yesilyurt 10/21/2024

Quant Time: Oct 19 00:29:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 19 00:23:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	46983	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	50408	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	21792	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	9162	12.406	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	49.640%		
7) Chloroethane-d5	2.893	69	10803	19.325	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.320%		
11) 1,1-Dichloroethene-d2	4.027	65	3863	12.576	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	50.320%		
21) 2-Butanone-d5	7.094	46	6225m	46.839	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.680%		
24) Chloroform-d	7.648	84	31336	23.322	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.280%		
26) 1,2-Dichloroethane-d4	8.307	65	18456m	26.415	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	105.680%		
32) Benzene-d6	8.276	84	42075	14.381	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	57.520%		
36) 1,2-Dichloropropane-d6	9.270	67	18293	21.303	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.200%		
41) Toluene-d8	10.325	98	30611	11.461	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	45.840%		
43) trans-1,3-Dichloroprop...	10.581	79	6020	16.742	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.960%		
47) 2-Hexanone-d5	10.922	63	4451	40.244	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.480%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	17821	28.259	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	113.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152	15943	21.622	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	86.480%		
Target Compounds					Qvalue	
13) Acetone	4.131	43	3996m	20.537	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030669.D
Acq On : 18 Oct 2024 17:05
Operator : SY/MD
Sample : P4414-21RE
Misc : 5.79g/10mL/MSVOA_W/SOIL/B
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4F82RE

Quant Time: Oct 19 00:29:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 19 00:23:37 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

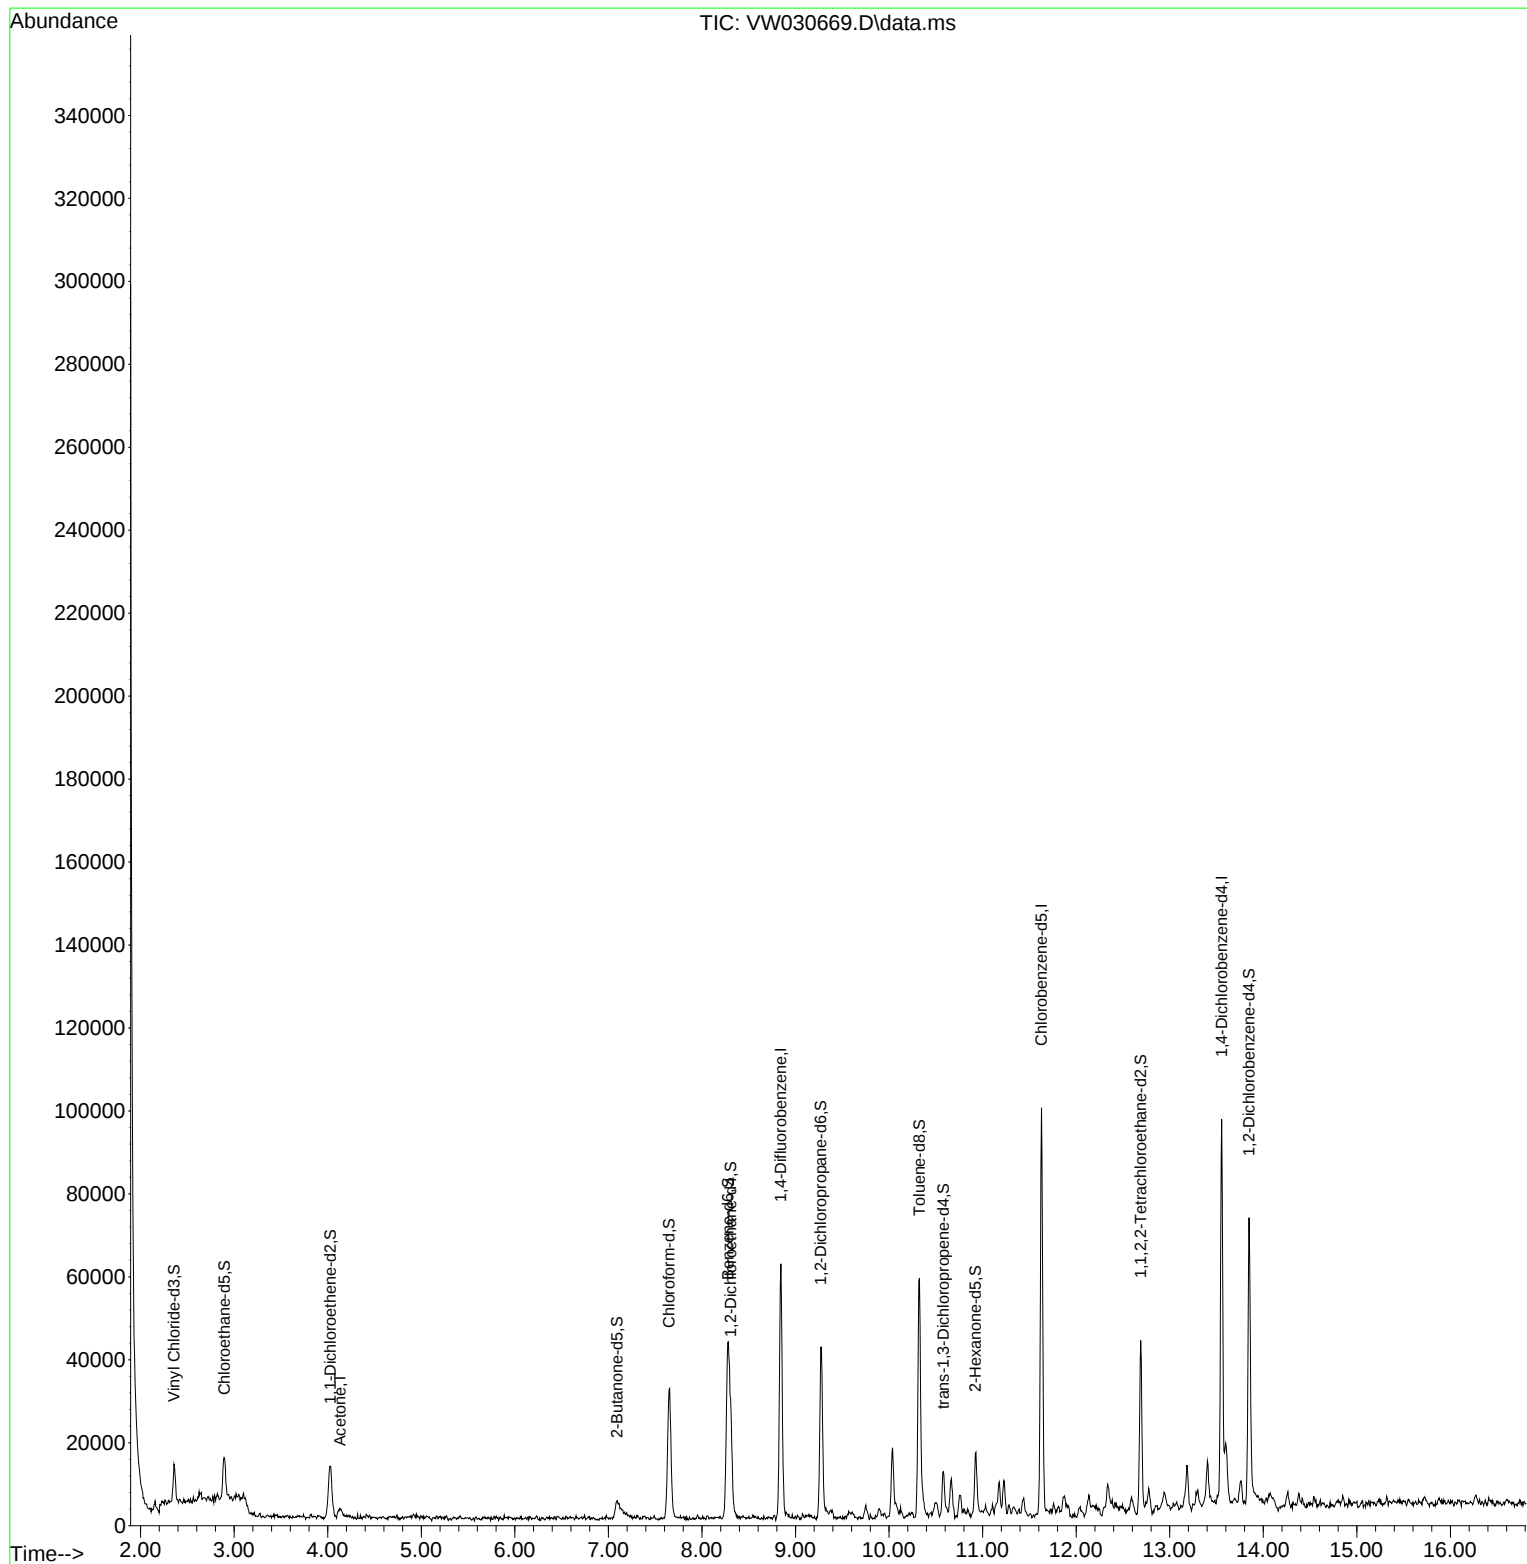

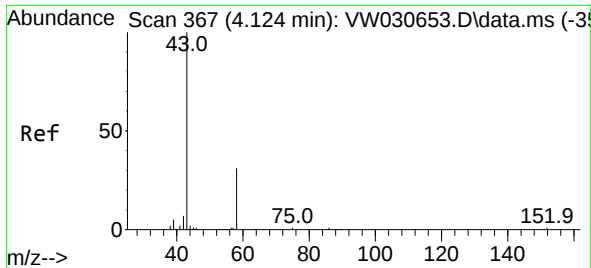

#13
Acetone
Concen: 20.537 ug/L m
RT: 4.131 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW030669.D
Acq: 18 Oct 2024 17:05

Instrument :
MSVOA_W
ClientSampleId :
A4F82RE

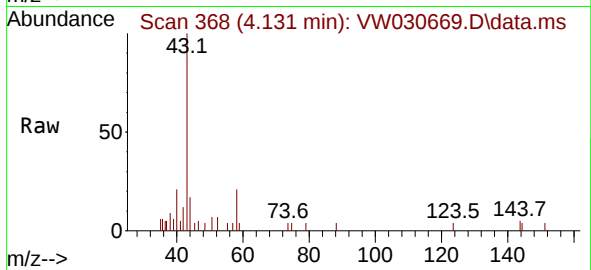

Tgt Ion: 43 Resp: 3990
Ion Ratio Lower Upper
43 100
58 15.1 0.0 57.6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/21/2024
Supervised By :Semsettin Yesilyurt 10/21/2024

