


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101824\
Data File : VW030652.D
Acq On : 18 Oct 2024 09:07
Operator : SY/MD
Sample : BFB579
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB579

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Sat Oct 19 00:23:37 2024

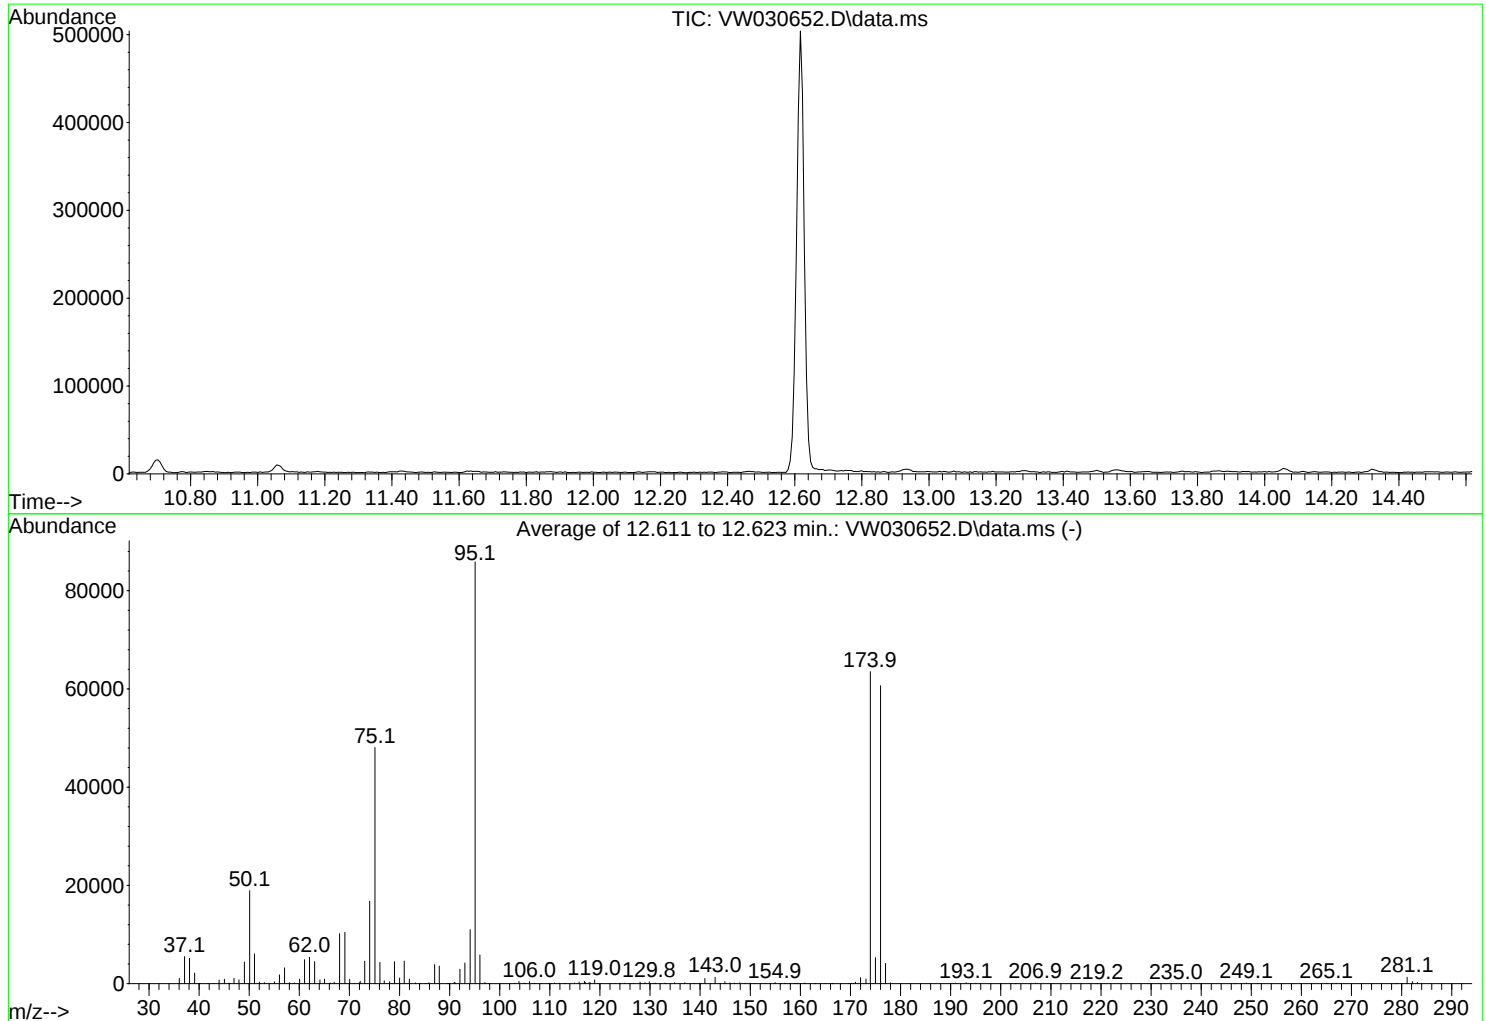

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	18925	PASS
75	95	30	80	56.0	48083	PASS
95	95	100	100	100.0	85880	PASS
96	95	5	9	6.8	5839	PASS
173	174	0.00	2	1.5	936	PASS
174	95	50	120	74.0	63517	PASS
175	174	5	9	8.3	5265	PASS
176	174	95	101	95.5	60661	PASS
177	176	5	9	6.8	4137	PASS

m/z	Abundance
35.20	53.0
37.80	68.0
38.10	76.0
39.10	107.0
40.00	338.0
41.30	127.0
42.40	53.0
42.90	80.0
44.00	177.0
47.60	52.0
48.40	77.0
49.50	52.0
52.80	55.0
64.70	56.0
65.80	52.0
74.00	51.0
83.80	55.0
123.50	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
36.00	1144.0
37.10	5244.0
38.10	5254.0
39.10	2520.0
40.00	362.0
41.90	75.0
43.00	158.0
44.00	996.0
45.00	1036.0
46.00	153.0
47.00	1029.0
48.00	856.0
49.00	4330.0
50.10	18568.0
51.10	6118.0
52.20	265.0
53.00	200.0
53.90	103.0
55.00	318.0
56.10	1668.0
57.00	3286.0
58.00	156.0
59.00	164.0
60.00	852.0
61.10	4571.0
62.10	5314.0
63.00	4240.0
64.10	1016.0
65.10	1204.0
66.10	207.0
67.00	374.0
68.00	10118.0
69.10	9974.0
70.10	757.0
72.00	563.0
73.00	4394.0
74.10	14999.0
75.10	45608.0
76.10	4064.0
77.00	555.0
78.10	372.0
79.00	4192.0
80.00	1162.0
81.00	4793.0
81.90	852.0
83.10	135.0
85.10	90.0
85.90	177.0
87.00	3592.0
88.00	3260.0
91.20	383.0
92.10	2621.0
93.10	3937.0
94.10	10968.0
95.10	76552.0
96.10	5558.0
97.10	279.0
102.90	129.0
103.80	389.0
104.90	225.0
105.90	398.0
107.10	144.0
108.20	63.0
109.90	88.0
111.10	161.0
111.90	121.0
112.90	93.0
115.00	201.0
115.80	384.0
116.90	695.0
117.90	437.0
118.90	888.0
124.00	75.0
125.00	119.0
125.80	81.0
128.10	317.0
129.00	138.0
129.80	290.0
131.00	177.0
133.00	196.0
134.90	192.0
136.90	196.0
138.90	70.0
140.00	115.0
140.90	904.0
143.00	1361.0
143.90	56.0
144.90	474.0
146.00	216.0
146.80	93.0
147.80	150.0
148.90	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

150.00	91.0
153.90	64.0
154.90	129.0
157.00	125.0
157.80	85.0
158.80	153.0
159.30	58.0
161.00	73.0
162.90	54.0
165.00	56.0
169.70	69.0
170.90	283.0
172.00	1160.0
173.10	1266.0
173.90	51936.0
175.00	4536.0
176.00	50008.0
177.00	3607.0
178.00	218.0
191.00	231.0
193.10	237.0
194.00	102.0
194.90	83.0
202.90	58.0
204.90	117.0
206.90	161.0
235.00	75.0
249.00	270.0
251.20	68.0
265.10	144.0
266.10	83.0
267.00	89.0
278.90	50.0
281.10	2197.0
282.20	662.0
283.10	261.0
284.10	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
36.00	1158.0
37.10	6381.0
38.10	6011.0
39.10	2382.0
39.90	395.0
41.70	51.0
42.90	182.0
44.10	939.0
45.10	944.0
45.90	159.0
46.20	165.0
47.00	1293.0
48.00	853.0
49.10	4878.0
50.10	21224.0
51.10	6875.0
52.00	369.0
53.00	192.0
53.90	74.0
55.10	356.0
56.00	2058.0
57.10	3496.0
58.10	254.0
59.10	98.0
60.10	1056.0
61.00	5570.0
62.00	6242.0
63.10	5547.0
64.10	682.0
65.00	766.0
66.20	181.0
67.00	296.0
68.10	11032.0
69.10	12291.0
70.00	1081.0
71.10	64.0
72.20	681.0
73.10	5325.0
74.10	19944.0
75.10	55272.0
76.10	4972.0
76.90	545.0
77.90	335.0
79.00	5220.0
80.00	1189.0
81.00	4915.0
82.00	1089.0
83.10	168.0
85.30	85.0
85.90	247.0
87.00	4012.0
87.90	4028.0
90.90	447.0
92.00	3507.0
93.10	4608.0
94.10	11376.0
95.10	99480.0
96.00	6619.0
97.00	256.0
97.80	63.0
102.90	126.0
103.90	449.0
104.80	138.0
106.00	515.0
106.80	164.0
109.80	110.0
110.90	155.0
111.90	102.0
113.10	86.0
114.90	131.0
115.90	328.0
116.90	664.0
118.10	467.0
118.90	746.0
119.80	61.0
123.00	79.0
124.00	105.0
124.80	116.0
126.00	123.0
128.00	389.0
129.00	160.0
129.90	440.0
131.10	127.0
133.20	175.0
134.90	212.0
136.90	163.0
138.80	55.0
139.80	115.0
141.00	1232.0
143.00	1238.0
143.90	86.0
144.90	417.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

146.00	140.0
146.90	58.0
147.90	156.0
148.90	69.0
150.00	132.0
153.00	76.0
153.80	79.0
155.00	357.0
156.80	140.0
158.00	73.0
158.80	147.0
160.90	160.0
165.00	76.0
166.30	51.0
170.30	111.0
171.00	461.0
172.00	1357.0
173.10	1542.0
174.00	69232.0
175.00	5856.0
176.00	66424.0
177.00	4758.0
178.00	161.0
190.50	89.0
191.00	92.0
193.10	264.0
194.10	80.0
207.00	114.0
219.20	52.0
249.10	147.0
265.00	194.0
266.10	89.0
266.90	75.0
280.10	70.0
281.10	995.0
282.10	379.0
283.20	309.0
283.90	116.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

m/z	Abundance
36.10	929.0
37.10	4878.0
38.10	4422.0
39.10	1890.0
40.10	314.0
41.60	65.0
42.90	64.0
44.00	772.0
45.00	729.0
46.10	118.0
46.90	931.0
47.90	664.0
49.10	4016.0
50.10	16984.0
51.00	5229.0
52.00	347.0
53.10	160.0
55.00	432.0
56.00	1703.0
57.10	2934.0
58.10	174.0
59.10	121.0
60.00	885.0
61.10	4527.0
62.10	4607.0
63.10	3687.0
64.00	558.0
65.00	739.0
66.20	110.0
66.90	355.0
68.10	9350.0
69.10	9132.0
70.00	815.0
71.00	88.0
72.10	697.0
73.10	4006.0
74.10	15573.0
75.10	43368.0
76.10	3945.0
77.00	674.0
78.10	446.0
79.00	3953.0
80.00	1122.0
80.90	4061.0
82.00	835.0
83.20	198.0
84.10	75.0
85.80	159.0
87.00	4022.0
88.00	3514.0
89.60	56.0
91.00	433.0
92.10	2683.0
93.00	4049.0
94.10	10566.0
95.10	81608.0
96.10	5341.0
97.00	185.0
103.00	81.0
103.90	545.0
105.10	113.0
106.00	394.0
106.90	170.0
109.90	82.0
110.40	107.0
110.90	167.0
111.90	92.0
113.10	153.0
114.90	144.0
115.90	283.0
117.10	717.0
117.80	296.0
119.00	642.0
119.80	52.0
123.00	52.0
124.00	104.0
124.80	69.0
126.70	64.0
127.90	299.0
129.00	294.0
129.90	413.0
130.90	122.0
132.80	94.0
134.90	193.0
137.00	277.0
138.90	60.0
139.70	71.0
140.20	124.0
141.00	1008.0
142.10	153.0
143.00	1358.0
144.10	115.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579

145.00	369.0
145.80	133.0
146.90	121.0
148.00	231.0
149.00	124.0
150.00	118.0
150.80	63.0
153.00	59.0
154.00	91.0
155.00	254.0
156.00	56.0
157.10	138.0
159.00	114.0
160.80	135.0
170.20	97.0
170.60	144.0
171.10	182.0
172.00	1133.0
174.00	69384.0
175.00	5403.0
176.00	65552.0
177.00	4045.0
178.00	104.0
191.00	105.0
193.10	131.0
207.00	59.0
207.30	59.0
246.70	58.0
281.00	708.0
282.10	266.0
283.10	156.0

Instrument :
MSVOA_W
ClientSampleId :
BFB579