

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
 Data File : VW024937.D
 Acq On : 19 Oct 2022 14:36
 Operator : SY/VA
 Sample : VW1019SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK429

Quant Time: Oct 20 01:59:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 20 01:56:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	427587	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	382028	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	184899	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	113318	22.464	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.840%		
7) Chloroethane-d5	2.885	69	66346	22.463	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.840%		
11) 1,1-Dichloroethene-d2	4.019	63	183940	16.770	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.080%		
21) 2-Butanone-d5	7.079	46	78693	49.233	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.460%		
24) Chloroform-d	7.653	84	292027	24.214	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.840%		
26) 1,2-Dichloroethane-d4	8.305	65	153519	24.322	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.280%		
32) Benzene-d6	8.274	84	596188	24.887	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.560%		
36) 1,2-Dichloropropane-d6	9.274	67	185479	25.243	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.960%		
41) Toluene-d8	10.323	98	532493	24.765	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	99.080%		
43) trans-1,3-Dichloroprop...	10.579	79	72289	25.941	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	103.760%		
47) 2-Hexanone-d5	10.926	63	61664	50.057	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.120%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	142131	24.804	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.200%		
66) 1,2-Dichlorobenzene-d4	13.853	152	170546	25.240	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.960%		
Target Compounds						Qvalue
34) Trichloroethene	8.841	95	12989	1.984	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
Data File : VW024937.D
Acq On : 19 Oct 2022 14:36
Operator : SY/VA
Sample : VW1019SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK429


Quant Time: Oct 20 01:59:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 20 01:56:31 2022
Response via : Initial Calibration

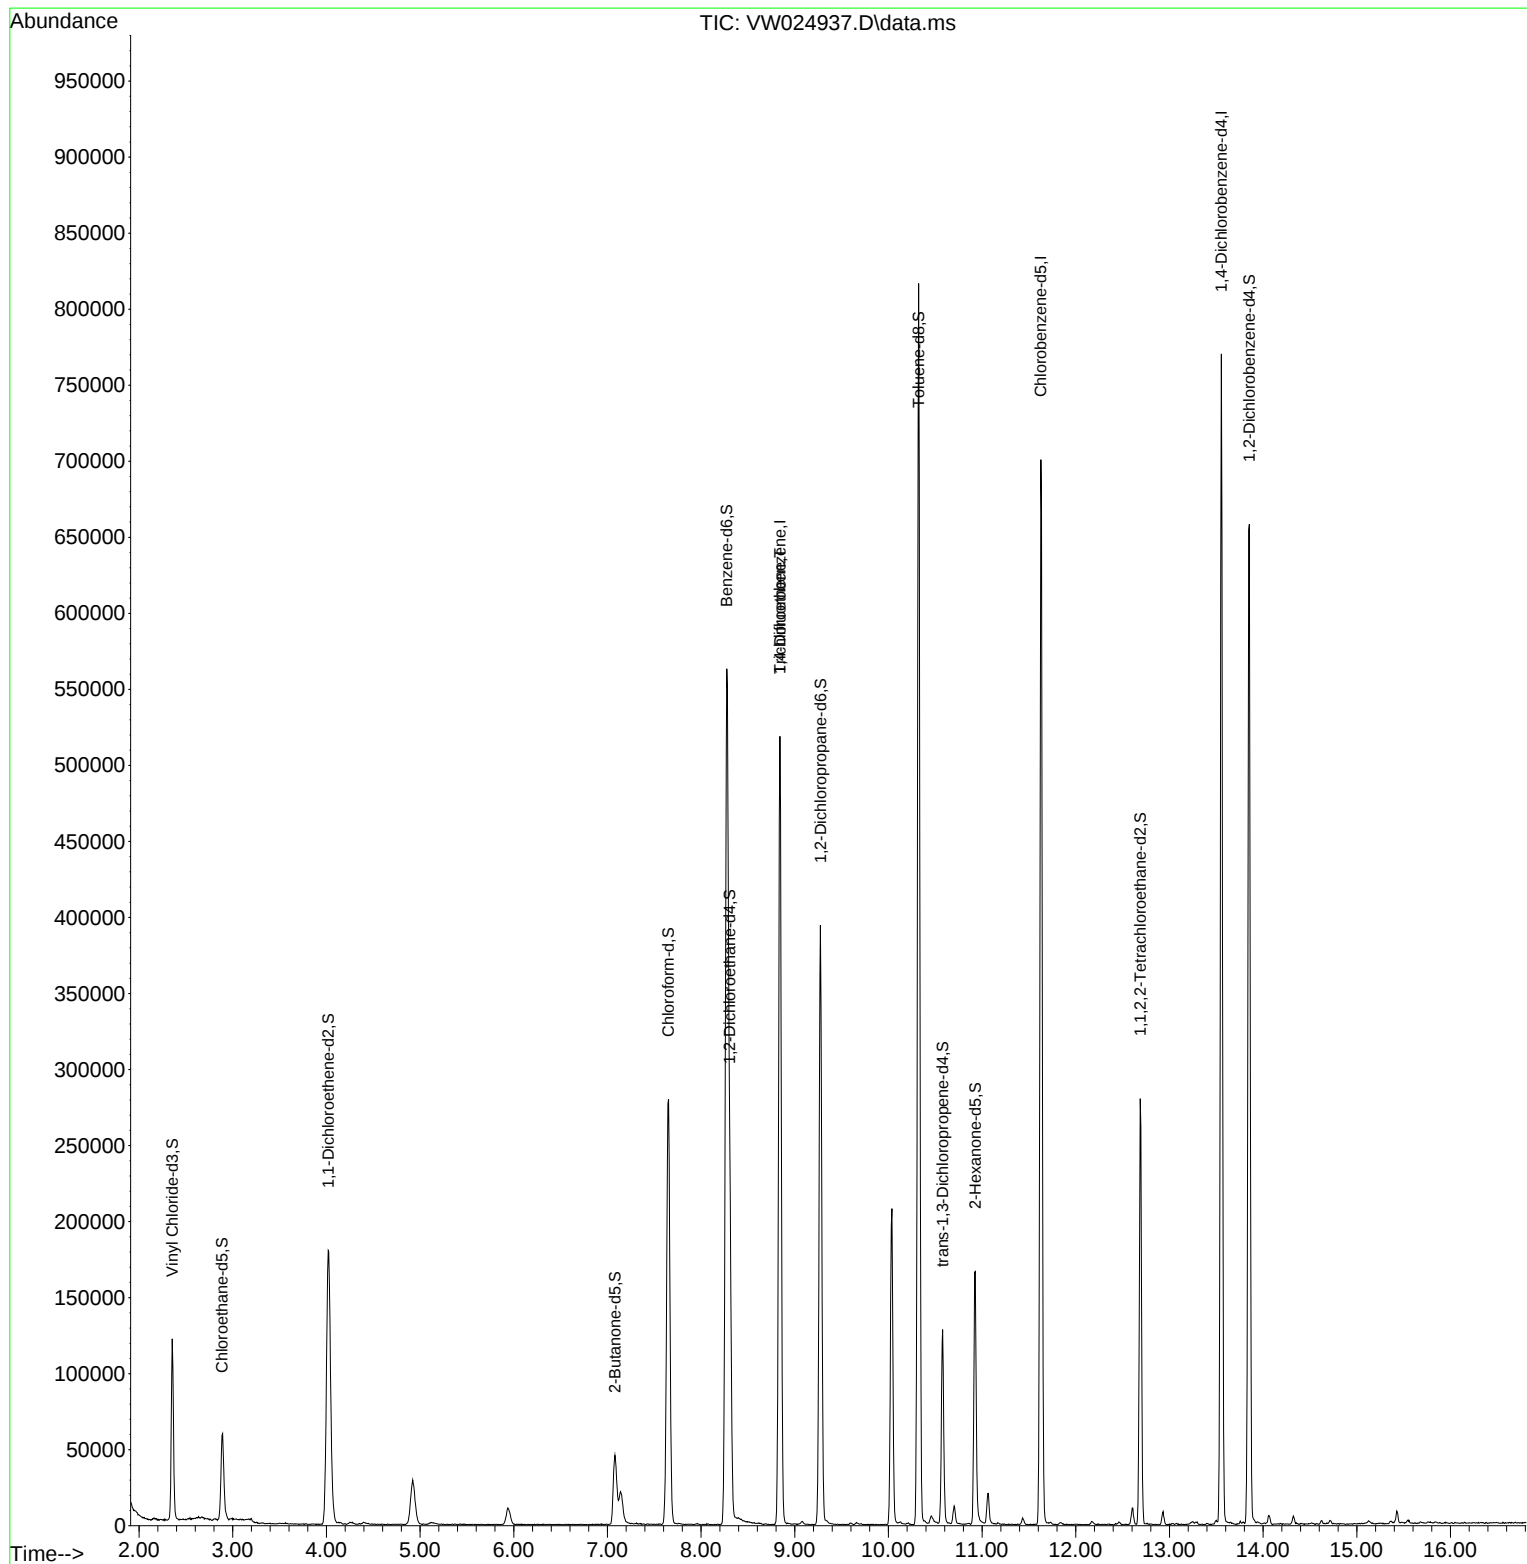

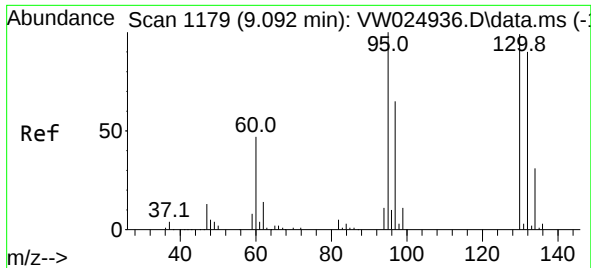

#34
 Trichloroethene
 Concen: 1.984 ug/L
 RT: 8.841 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW024937.D
 Acq: 19 Oct 2022 14:36

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK429

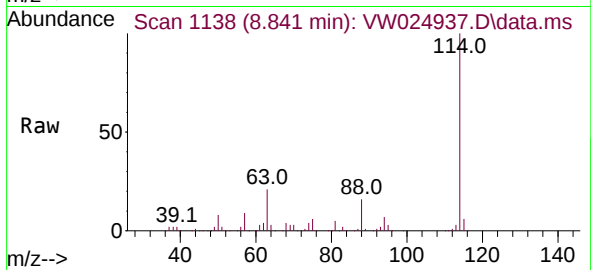

Tgt Ion: 95	Resp: 12989
Ion Ratio	Lower Upper
95	100
97	0.0 44.2 82.0#
132	0.0 62.9 116.7#
130	0.0 66.8 124.0#

