

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
 Data File : VW024952.D
 Acq On : 19 Oct 2022 21:11
 Operator : SY/VA
 Sample : N5193-03
 Misc : 4.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LSP-SS-02-01-03

Quant Time: Oct 20 02:04:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 20 01:56:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	514547	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	378655	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	111815	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	103515	17.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.200%
7) Chloroethane-d5	2.885	69	67028	18.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.440%
11) 1,1-Dichloroethene-d2	4.019	63	174185	13.197	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.800%
21) 2-Butanone-d5	7.080	46	124610	64.785	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.580%
24) Chloroform-d	7.647	84	342422	23.594	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.360%
26) 1,2-Dichloroethane-d4	8.305	65	186356	24.535	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.120%
32) Benzene-d6	8.275	84	644946	27.162	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.640%
36) 1,2-Dichloropropane-d6	9.274	67	215771	29.628	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	118.520%
41) Toluene-d8	10.323	98	486406	22.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.280%
43) trans-1,3-Dichloroprop...	10.579	79	75192	27.223	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	108.880%
47) 2-Hexanone-d5	10.920	63	95055	77.849	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	155.700%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	154362	27.179	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.720%
66) 1,2-Dichlorobenzene-d4	13.847	152	93336	22.842	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.360%
Target Compounds					Qvalue	
13) Acetone	4.123	43	20100	14.934	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
Data File : VW024952.D
Acq On : 19 Oct 2022 21:11
Operator : SY/VA
Sample : N5193-03
Misc : 4.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LSP-SS-02-01-03

Quant Time: Oct 20 02:04:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 20 01:56:31 2022
Response via : Initial Calibration

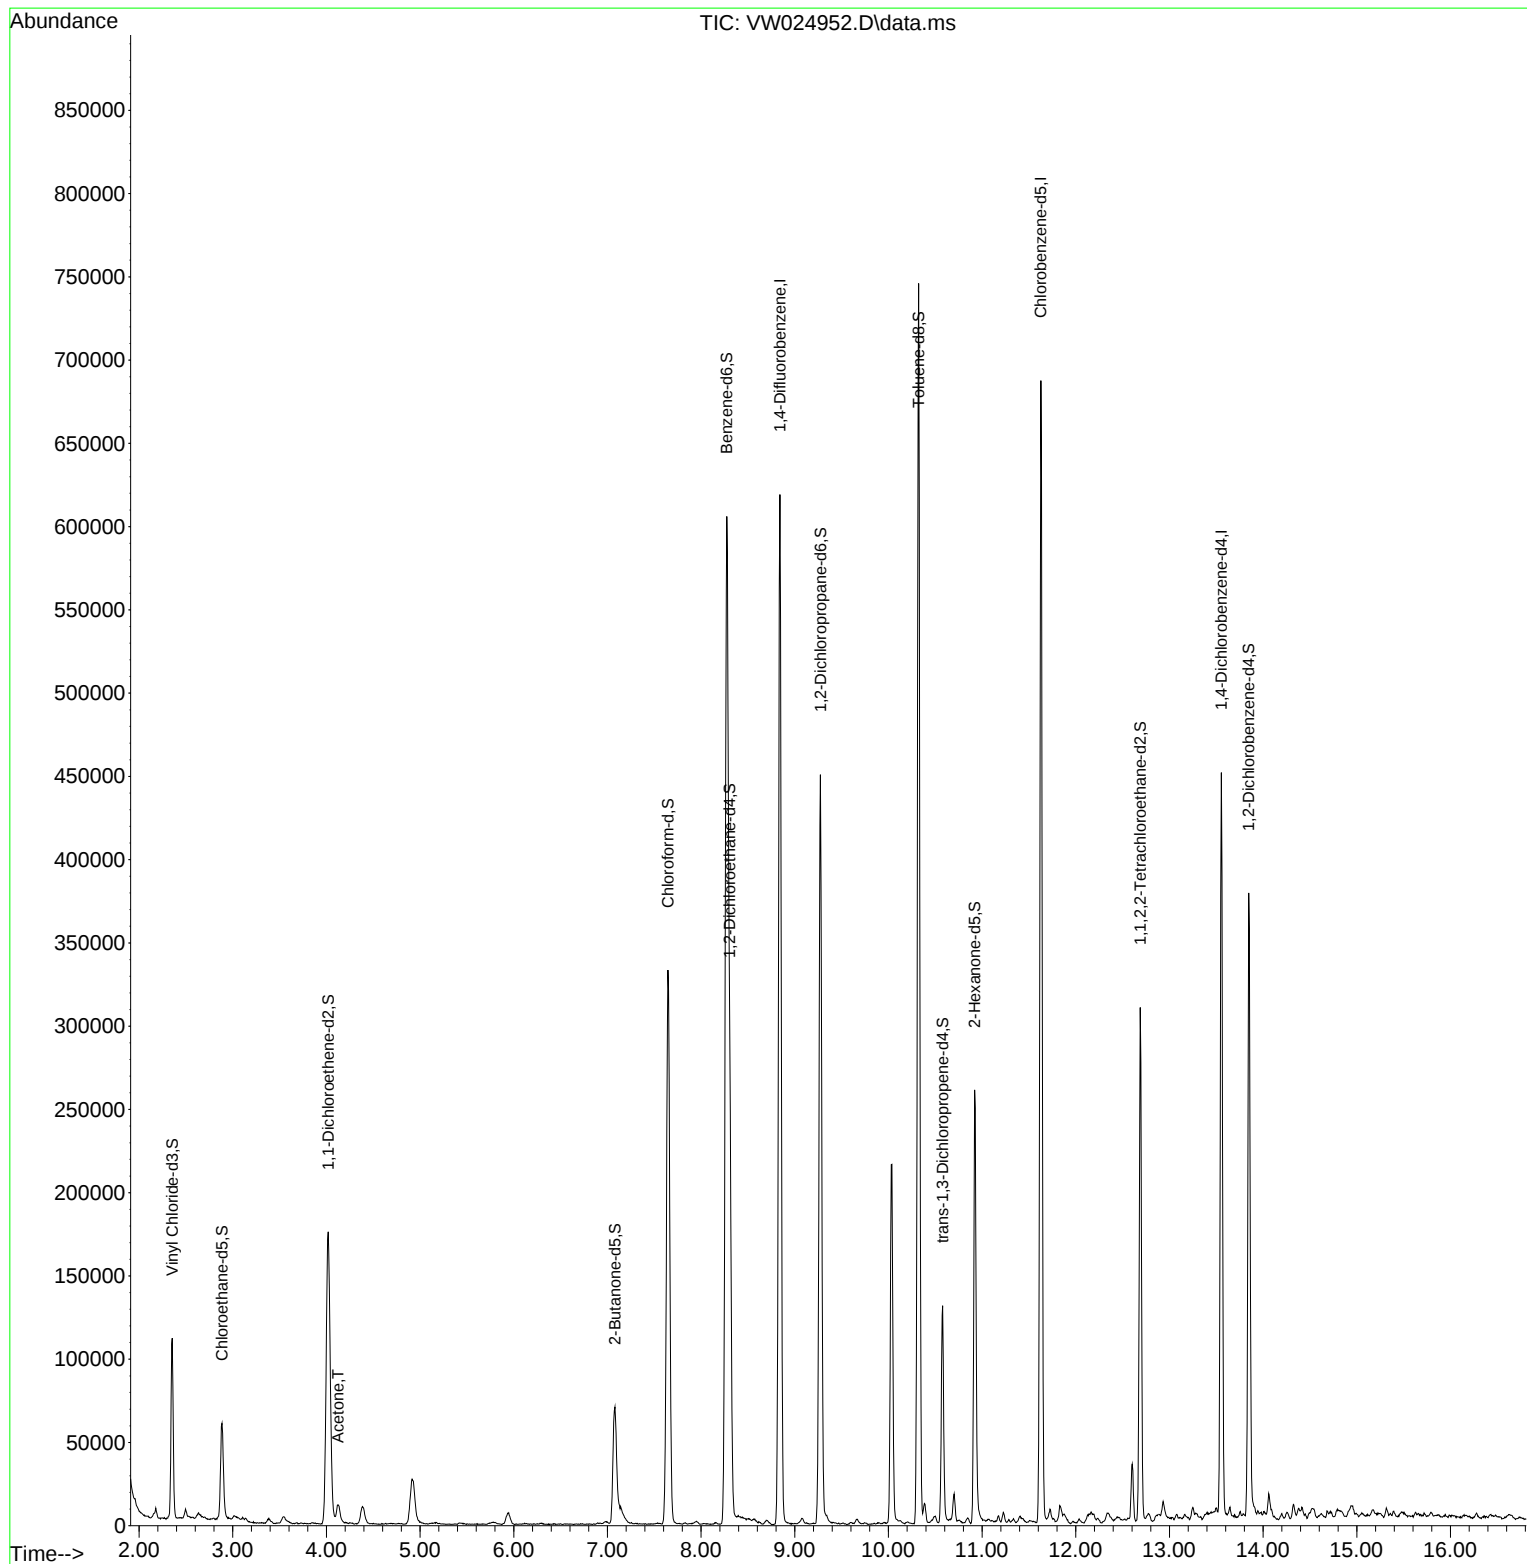

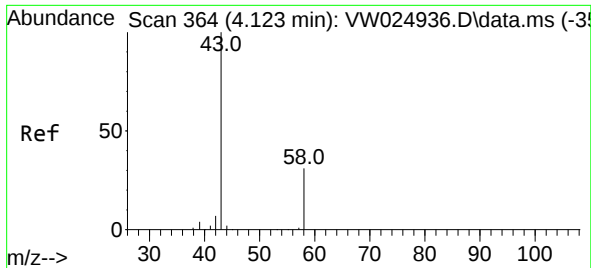

#13
 Acetone
 Concen: 14.934 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW024952.D
 Acq: 19 Oct 2022 21:11

Instrument :
 MSVOA_W
 ClientSampleId :
 LSP-SS-02-01-03

Tgt Ion: 43 Resp: 20100
 Ion Ratio Lower Upper
 43 100
 58 33.8 0.0 64.2

