




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
Data File : VW024955.D
Acq On : 19 Oct 2022 22:23
Operator : SY/VA
Sample : N5193-06
Misc : 6.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LSP-SS-03-03-05

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2022
Supervised By :Mahesh Dadoda 10/20/2022

Quant Time: Oct 20 02:04:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 20 01:56:31 2022
Response via : Initial Calibration

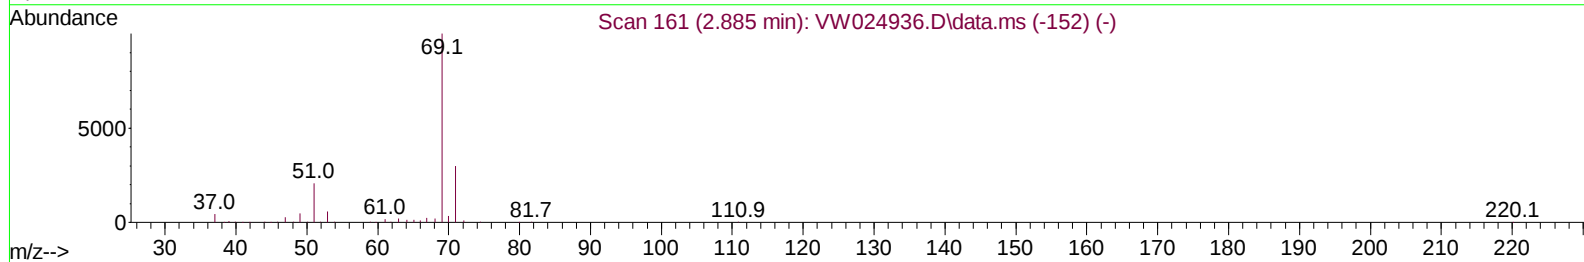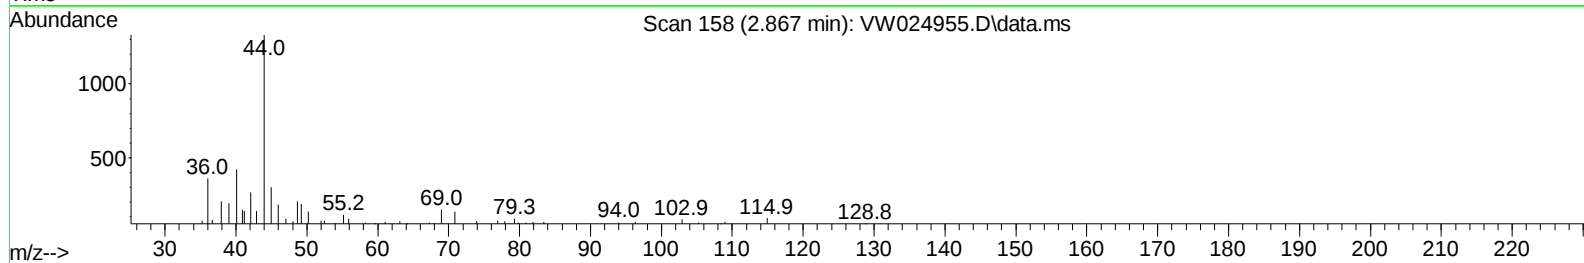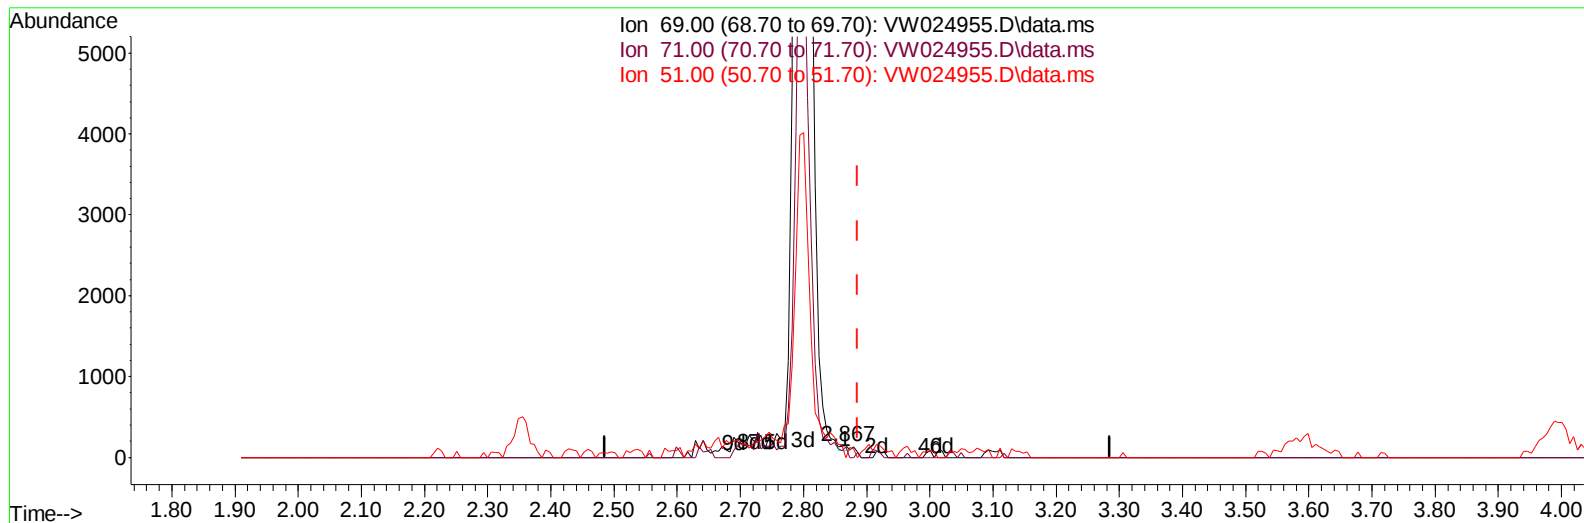

TIC: VW024955.D\data.ms

(7) Chloroethane-d5 (S)

2.867min (-0.018) 0.02 ug/L

response 44

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.50	111.36#
51.00	29.30	193.18#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
 Data File : VW024955.D
 Acq On : 19 Oct 2022 22:23
 Operator : SY/VA
 Sample : N5193-06
 Misc : 6.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LSP-SS-03-03-05

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2022
 Supervised By :Mahesh Dadoda 10/20/2022

Quant Time: Oct 20 02:04:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 20 01:56:31 2022
 Response via : Initial Calibration

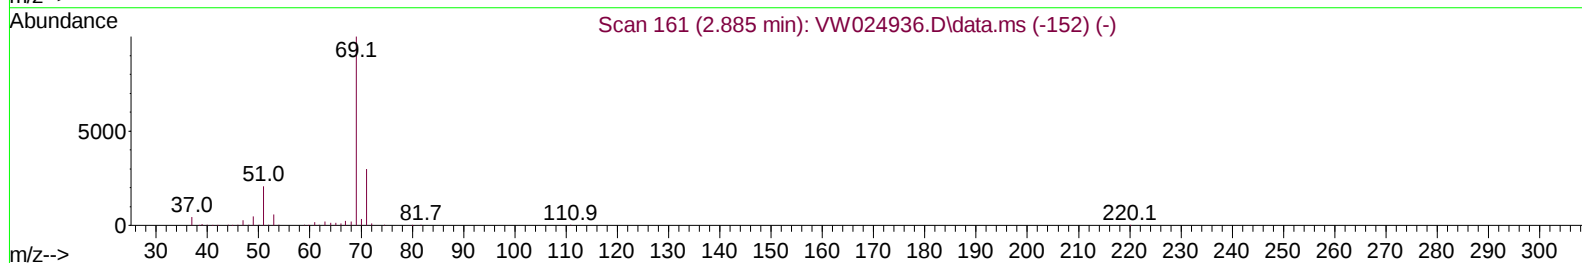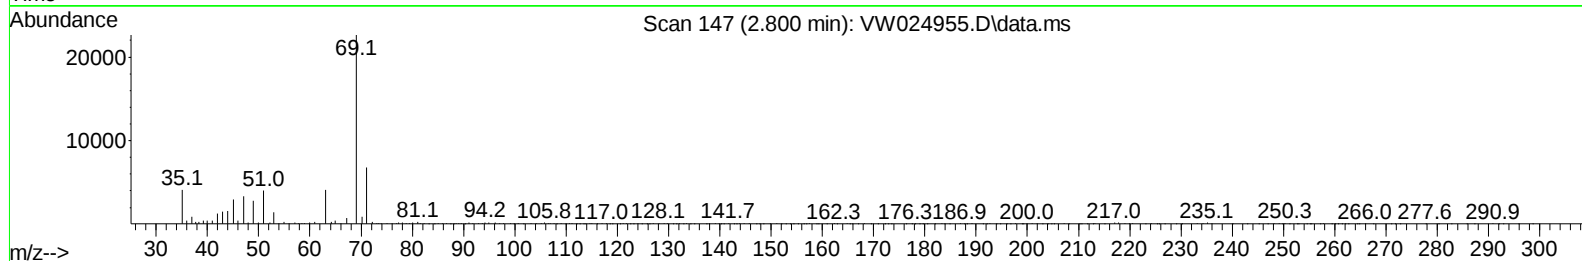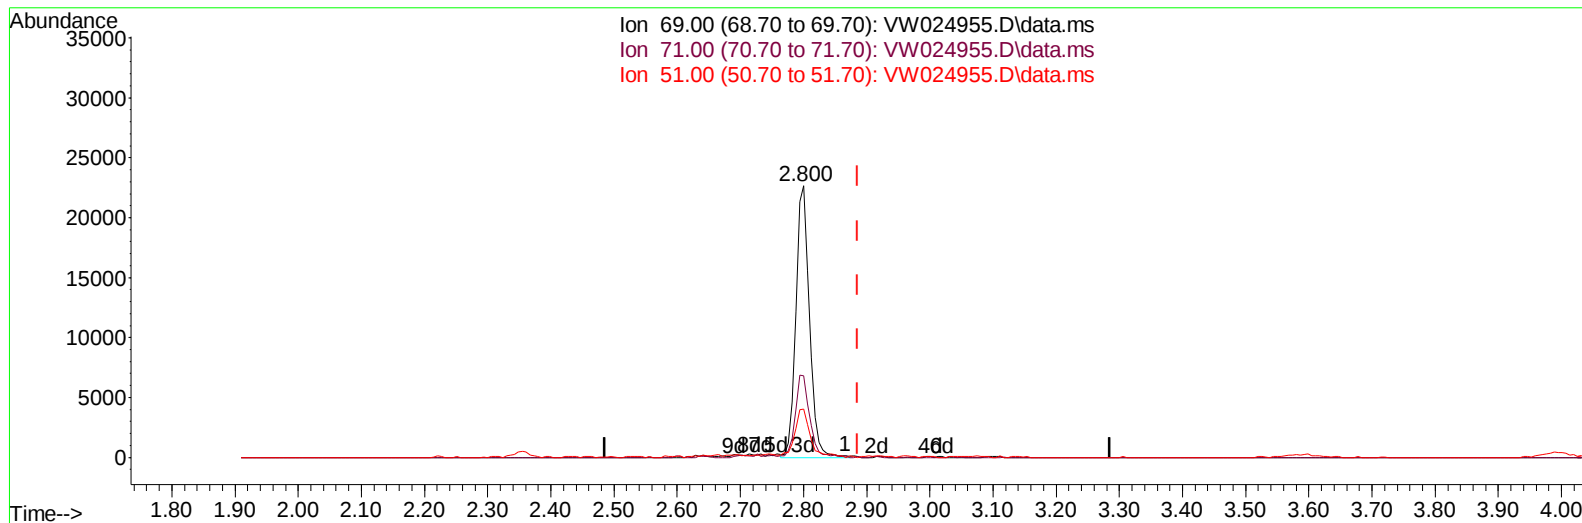

TIC: VW024955.D\data.ms

(7) Chloroethane-d5 (S)

2.800min (-0.085) 11.81 ug/L m

response 33898

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.50	0.14#
51.00	29.30	0.25#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101922\
 Data File : VW024955.D
 Acq On : 19 Oct 2022 22:23
 Operator : SY/VA
 Sample : N5193-06
 Misc : 6.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LSP-SS-03-03-05

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2022
 Supervised By :Mahesh Dadoda 10/20/2022

Quant Time: Oct 20 02:04:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 20 01:56:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	415511	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	333545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	108062	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	92842	18.939	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.760%	
7) Chloroethane-d5	2.800	69	33898m	11.811	ug/L	-0.09
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.240%	
11) 1,1-Dichloroethene-d2	3.989	63	135073	12.673	ug/L	-0.04
Spiked Amount 25.000	Range 45	- 110	Recovery	=	50.680%	
21) 2-Butanone-d5	7.086	46	127092	81.825	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	163.640%#	
24) Chloroform-d	7.641	84	283700	24.207	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.840%	
26) 1,2-Dichloroethane-d4	8.299	65	163184	26.605	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	106.400%	
32) Benzene-d6	8.268	84	539502	25.794	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	103.160%	
36) 1,2-Dichloropropane-d6	9.268	67	190908	29.759	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	119.040%	
41) Toluene-d8	10.317	98	424304	22.602	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	10.579	79	54382	22.352	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.400%	
47) 2-Hexanone-d5	10.927	63	87216	81.090	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	162.180%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	166101	33.201	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	132.800%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	106599	26.994	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	107.960%	
Target Compounds					Qvalue	
13) Acetone	4.135	43	12183	11.209	ug/L	95
15) Methyl Acetate	4.665	43	35992	13.607	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
Data File : VW024955.D
Acq On : 19 Oct 2022 22:23
Operator : SY/VA
Sample : N5193-06
Misc : 6.12g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LSP-SS-03-03-05

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2022
Supervised By :Mahesh Dadoda 10/20/2022

Quant Time: Oct 20 02:04:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 20 01:56:31 2022
Response via : Initial Calibration

