

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
 Data File : VW024949.D
 Acq On : 19 Oct 2022 19:58
 Operator : SY/VA
 Sample : N4757-11
 Misc : 5.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBWK6

Quant Time: Oct 20 02:03:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 20 01:56:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	489954	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	408462	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	150662	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	94918	16.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.680%
7) Chloroethane-d5	2.885	69	63434	18.743	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.960%
11) 1,1-Dichloroethene-d2	4.019	63	161424	12.844	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.360%
21) 2-Butanone-d5	7.074	46	113253	61.836	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.680%
24) Chloroform-d	7.647	84	321267	23.248	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	8.305	65	177381	24.525	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.120%
32) Benzene-d6	8.275	84	613150	23.938	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.760%
36) 1,2-Dichloropropane-d6	9.274	67	206288	26.259	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.040%
41) Toluene-d8	10.323	98	492677	21.431	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.720%
43) trans-1,3-Dichloroprop...	10.579	79	73032	24.512	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.040%
47) 2-Hexanone-d5	10.920	63	85346	64.797	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.600%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	173417	28.305	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	125862	22.860	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.440%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	40216	4.649	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
Data File : VW024949.D
Acq On : 19 Oct 2022 19:58
Operator : SY/VA
Sample : N4757-11
Misc : 5.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBWK6


Quant Time: Oct 20 02:03:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 20 01:56:31 2022
Response via : Initial Calibration

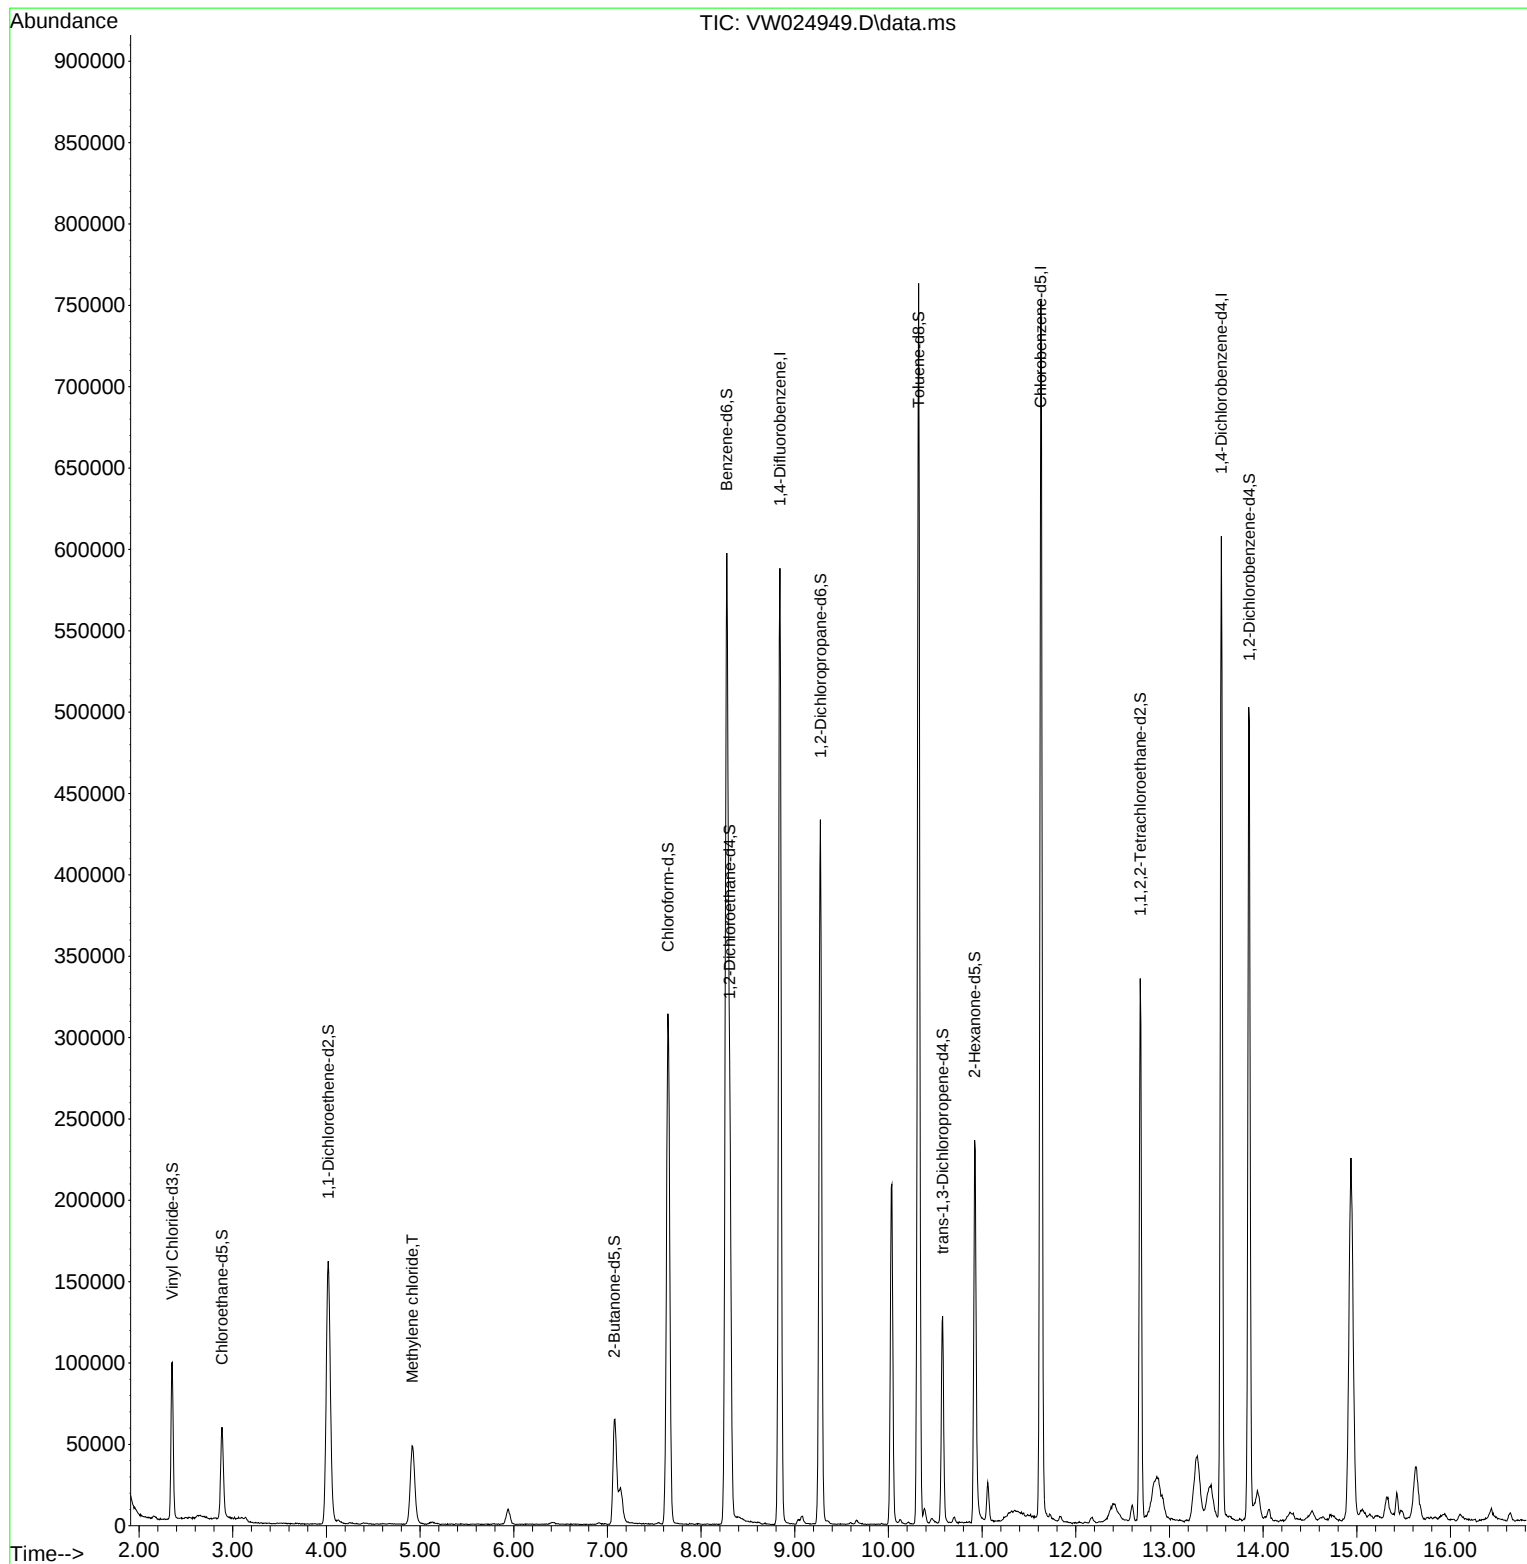

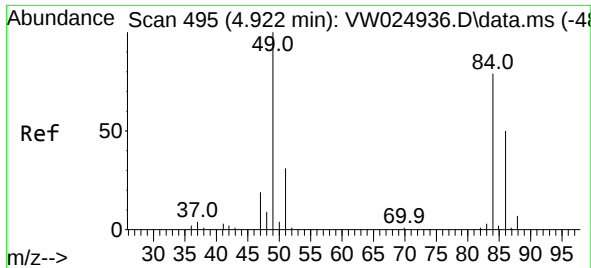

#16
Methylene chloride
Concen: 4.649 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW024949.D
Acq: 19 Oct 2022 19:58

Instrument :
MSVOA_W
ClientSampleId :
DBWK6

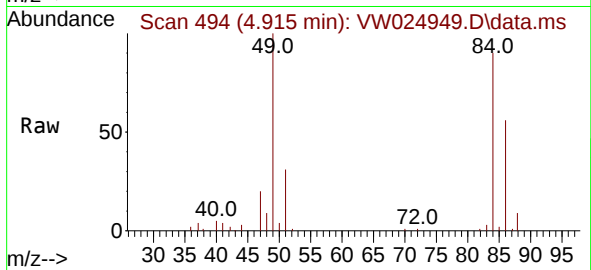

Tgt Ion: 84 Resp: 40216
Ion Ratio Lower Upper
84 100
86 62.5 45.5 84.5
49 111.6 90.9 168.9

