
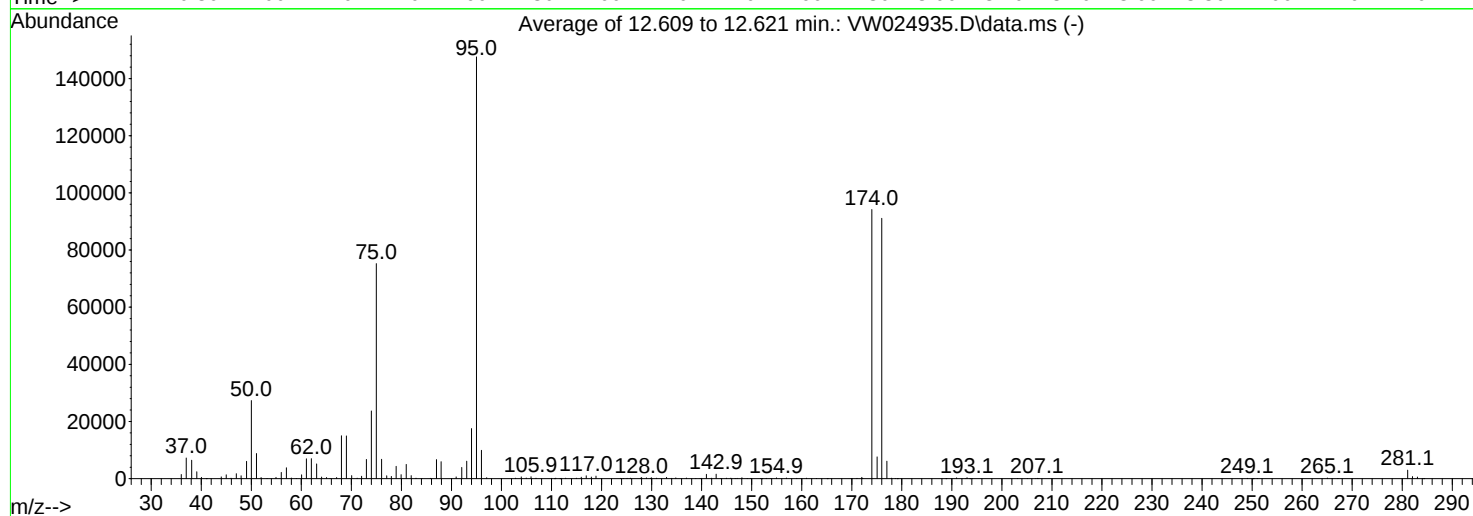


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101922\
 Data File : VW024935.D
 Acq On : 19 Oct 2022 12:36
 Operator : SY/VA
 Sample : BFB444
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB444

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Title : SFAM01.0
 Last Update : Thu Oct 20 01:56:31 2022

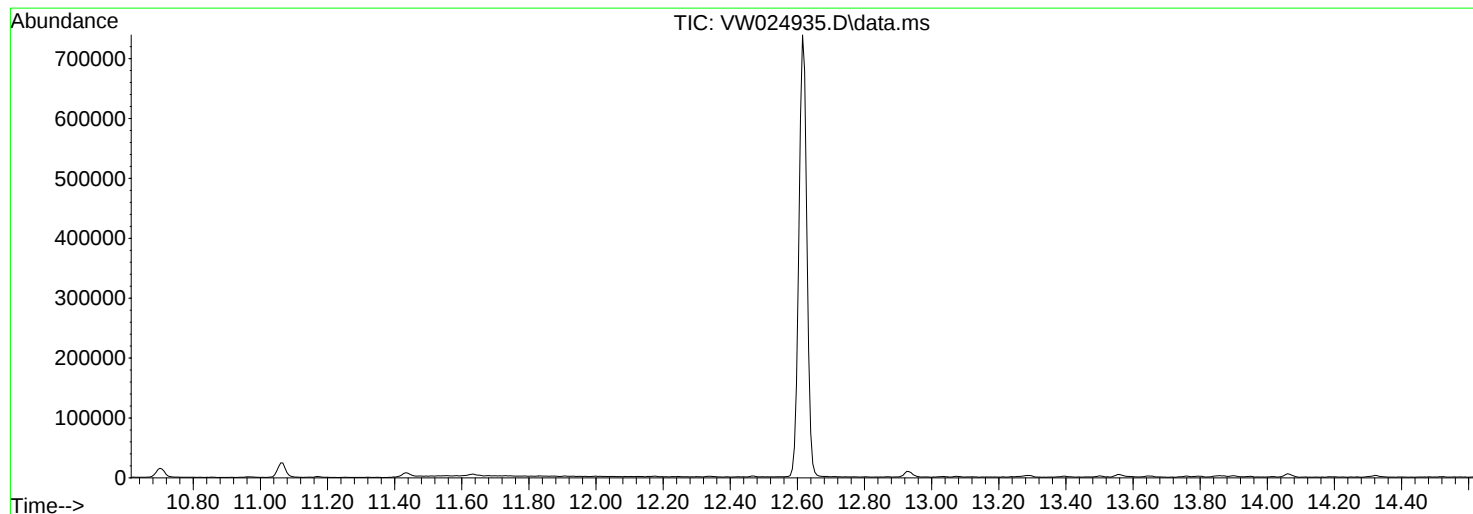

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	27355	PASS
75	95	30	80	51.0	75277	PASS
95	95	100	100	100.0	147605	PASS
96	95	5	9	6.7	9896	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.8	94195	PASS
175	174	5	9	8.1	7607	PASS
176	174	95	105	96.7	91085	PASS
177	176	5	10	6.7	6134	PASS

m/z	Abundance
36.00	362.0
36.90	91.0
37.90	144.0
39.90	638.0
40.90	90.0
43.10	186.0
44.00	258.0
45.00	82.0
56.00	81.0
57.00	76.0
70.90	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
36.00	1851.0
37.00	7167.0
38.10	6498.0
39.10	2417.0
39.90	632.0
41.10	91.0
43.90	718.0
45.10	1425.0
46.10	135.0
47.00	1767.0
47.90	1000.0
49.00	5604.0
50.00	25952.0
51.00	8129.0
52.00	320.0
53.20	61.0
55.00	415.0
56.00	1911.0
57.10	3712.0
58.00	263.0
59.00	63.0
60.10	1020.0
61.00	6226.0
62.00	6101.0
63.10	4755.0
64.00	650.0
65.10	375.0
67.00	427.0
68.00	14069.0
69.00	13332.0
70.00	896.0
71.10	97.0
72.00	735.0
73.00	6371.0
74.00	23080.0
75.00	69616.0
76.10	6240.0
77.00	888.0
78.10	804.0
78.90	3584.0
80.00	1342.0
81.00	4791.0
82.00	1006.0
82.80	126.0
84.10	56.0
87.00	5833.0
87.90	5118.0
90.90	538.0
92.00	3688.0
93.00	5442.0
94.00	15695.0
95.00	133952.0
96.00	8802.0
97.00	360.0
102.80	205.0
104.00	442.0
104.90	244.0
105.90	790.0
107.00	167.0
110.10	87.0
110.60	79.0
111.00	135.0
111.70	89.0
112.90	141.0
114.90	256.0
116.00	458.0
116.90	922.0
118.00	489.0
118.90	794.0
123.90	86.0
125.00	143.0
125.80	113.0
127.80	501.0
128.90	265.0
129.80	282.0
131.00	105.0
132.90	529.0
134.00	180.0
134.90	209.0
137.00	245.0
138.90	98.0
139.90	139.0
140.90	1266.0
141.90	182.0
142.90	1338.0
143.90	146.0
144.90	148.0
145.90	213.0
146.70	120.0
147.20	89.0
148.10	380.0
149.10	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

149.90	59.0
153.00	84.0
153.80	102.0
154.90	256.0
156.90	185.0
159.00	87.0
160.90	218.0
163.00	92.0
165.10	73.0
171.10	97.0
172.10	649.0
174.00	79016.0
175.00	6650.0
176.00	69272.0
177.00	5263.0
177.90	241.0
178.70	62.0
179.10	83.0
191.00	440.0
193.10	556.0
194.10	128.0
203.10	114.0
205.10	125.0
207.10	334.0
249.00	199.0
250.20	71.0
251.00	150.0
265.00	449.0
266.00	124.0
267.10	130.0
281.10	4576.0
282.00	1177.0
283.00	858.0
284.10	154.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
36.00	2019.0
37.10	8441.0
38.10	6684.0
39.10	2621.0
40.10	668.0
41.10	179.0
43.10	122.0
44.00	963.0
45.00	1400.0
45.90	292.0
47.00	1838.0
48.00	1059.0
49.00	7057.0
50.00	30416.0
51.00	9848.0
51.90	441.0
53.10	66.0
55.00	478.0
56.00	2752.0
57.00	4047.0
58.10	193.0
60.00	1627.0
61.00	8184.0
62.00	7946.0
63.00	5676.0
64.00	516.0
65.00	457.0
65.80	66.0
67.10	458.0
68.00	15952.0
69.00	17024.0
70.10	1226.0
71.10	241.0
72.10	899.0
73.00	7263.0
74.00	25584.0
75.00	84792.0
76.00	7613.0
77.10	1060.0
78.00	814.0
79.00	4933.0
79.90	1495.0
81.00	5406.0
81.90	1196.0
82.90	229.0
84.10	64.0
85.80	205.0
87.00	7524.0
88.00	6763.0
91.00	704.0
92.10	4058.0
93.00	7015.0
94.00	19552.0
95.00	167040.0
96.00	11613.0
97.10	351.0
102.90	120.0
103.90	779.0
104.90	215.0
105.90	620.0
106.90	157.0
110.10	94.0
110.80	141.0
111.90	245.0
112.80	138.0
115.00	126.0
116.00	564.0
116.90	1174.0
118.00	678.0
118.90	968.0
123.80	88.0
124.40	56.0
125.10	89.0
125.60	129.0
125.90	101.0
128.00	654.0
129.00	368.0
130.00	567.0
131.00	295.0
133.00	451.0
134.00	159.0
134.90	338.0
136.90	214.0
138.80	59.0
140.00	110.0
141.00	1760.0
142.00	187.0
142.90	1749.0
143.70	63.0
145.00	177.0
145.90	189.0
147.20	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

148.10	288.0
149.10	83.0
149.90	160.0
151.80	106.0
152.90	84.0
153.80	61.0
154.90	325.0
156.90	307.0
159.10	125.0
161.00	139.0
163.00	62.0
169.90	50.0
171.10	184.0
171.90	626.0
174.00	99400.0
175.00	8795.0
176.00	94368.0
177.00	6772.0
178.00	222.0
178.70	53.0
188.80	51.0
190.90	296.0
193.00	475.0
193.60	64.0
194.10	126.0
203.20	75.0
206.80	105.0
207.40	125.0
249.10	220.0
251.10	102.0
265.10	189.0
266.00	111.0
267.20	111.0
281.10	2799.0
282.10	679.0
283.10	526.0
284.30	80.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
36.00	1592.0
37.00	6431.0
38.10	6185.0
39.10	2185.0
40.00	671.0
41.10	55.0
42.90	132.0
44.10	1025.0
45.00	1403.0
45.90	143.0
47.00	1644.0
48.00	1000.0
49.10	5496.0
50.00	25696.0
51.10	8480.0
52.00	365.0
54.90	380.0
56.10	2136.0
57.00	3894.0
57.90	204.0
59.00	67.0
60.00	1452.0
61.00	6442.0
62.00	6889.0
63.00	5053.0
64.10	482.0
65.00	330.0
65.70	80.0
67.00	304.0
68.00	14952.0
69.00	14521.0
70.00	1092.0
71.20	136.0
72.00	820.0
73.00	6476.0
74.00	22448.0
75.00	71424.0
76.00	6477.0
77.00	1033.0
77.90	714.0
78.90	4481.0
80.00	1298.0
80.90	4710.0
82.00	952.0
83.00	109.0
85.80	123.0
87.00	6587.0
87.90	5980.0
90.90	666.0
92.00	4007.0
93.10	5816.0
94.00	17360.0
95.00	141824.0
96.00	9273.0
97.10	275.0
102.90	111.0
103.90	603.0
105.00	254.0
105.90	642.0
106.80	111.0
109.90	110.0
110.80	197.0
111.90	139.0
112.80	235.0
114.90	159.0
115.80	490.0
117.00	877.0
117.90	519.0
118.90	996.0
123.80	92.0
124.30	53.0
125.20	117.0
125.80	134.0
128.00	555.0
128.90	257.0
129.90	462.0
131.00	164.0
133.10	316.0
133.90	66.0
134.80	290.0
136.90	271.0
139.70	102.0
140.00	93.0
141.00	1472.0
142.00	180.0
142.90	1701.0
144.90	163.0
145.80	169.0
147.00	171.0
147.90	388.0
149.80	173.0
152.00	94.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

152.90	186.0
153.90	58.0
155.00	298.0
157.00	256.0
158.90	203.0
160.80	112.0
161.10	120.0
162.90	65.0
171.00	117.0
172.20	592.0
174.00	104168.0
175.10	7375.0
176.00	109616.0
177.00	6367.0
177.80	91.0
191.00	146.0
192.80	153.0
206.80	78.0
207.20	60.0
265.20	97.0
281.10	1577.0
282.10	411.0
283.10	307.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444