

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101923\
 Data File : VW027346.D
 Acq On : 19 Oct 2023 14:26
 Operator : SY/MD
 Sample : 04953-01
 Misc : 3.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAS0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2023
 Supervised By :Mahesh Dadoda 10/20/2023

Quant Time: Oct 20 02:49:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 20 02:46:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	525085	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	385803	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	127048	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.368	65	142239	17.750	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.000%		
7) Chloroethane-d5	2.899	69	116179	20.191	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.760%		
11) 1,1-Dichloroethene-d2	4.021	65	72102	17.956	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.840%		
21) 2-Butanone-d5	7.081	46	81155	30.469	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	60.940%		
24) Chloroform-d	7.648	84	305218	19.503	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	78.000%		
26) 1,2-Dichloroethane-d4	8.306	65	170673m	20.302	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	81.200%		
32) Benzene-d6	8.276	84	625211	23.952	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.800%		
36) 1,2-Dichloropropane-d6	9.276	67	201946	25.330	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.320%		
41) Toluene-d8	10.324	98	490910	20.740	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.960%		
43) trans-1,3-Dichloroprop...	10.580	79	67171	18.479	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	73.920%		
47) 2-Hexanone-d5	10.922	63	63291	38.370	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.740%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	128889	21.668	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	86.680%		
66) 1,2-Dichlorobenzene-d4	13.848	152	84241	18.297	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	73.200%#		
Target Compounds					Qvalue	
13) Acetone	4.130	43	10527	4.576	ug/L	99
16) Methylene chloride	4.929	84	20851	2.169	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101923\
Data File : VW027346.D
Acq On : 19 Oct 2023 14:26
Operator : SY/MD
Sample : 04953-01
Misc : 3.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAS0

Quant Time: Oct 20 02:49:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 20 02:46:04 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2023
Supervised By :Mahesh Dadoda 10/20/2023

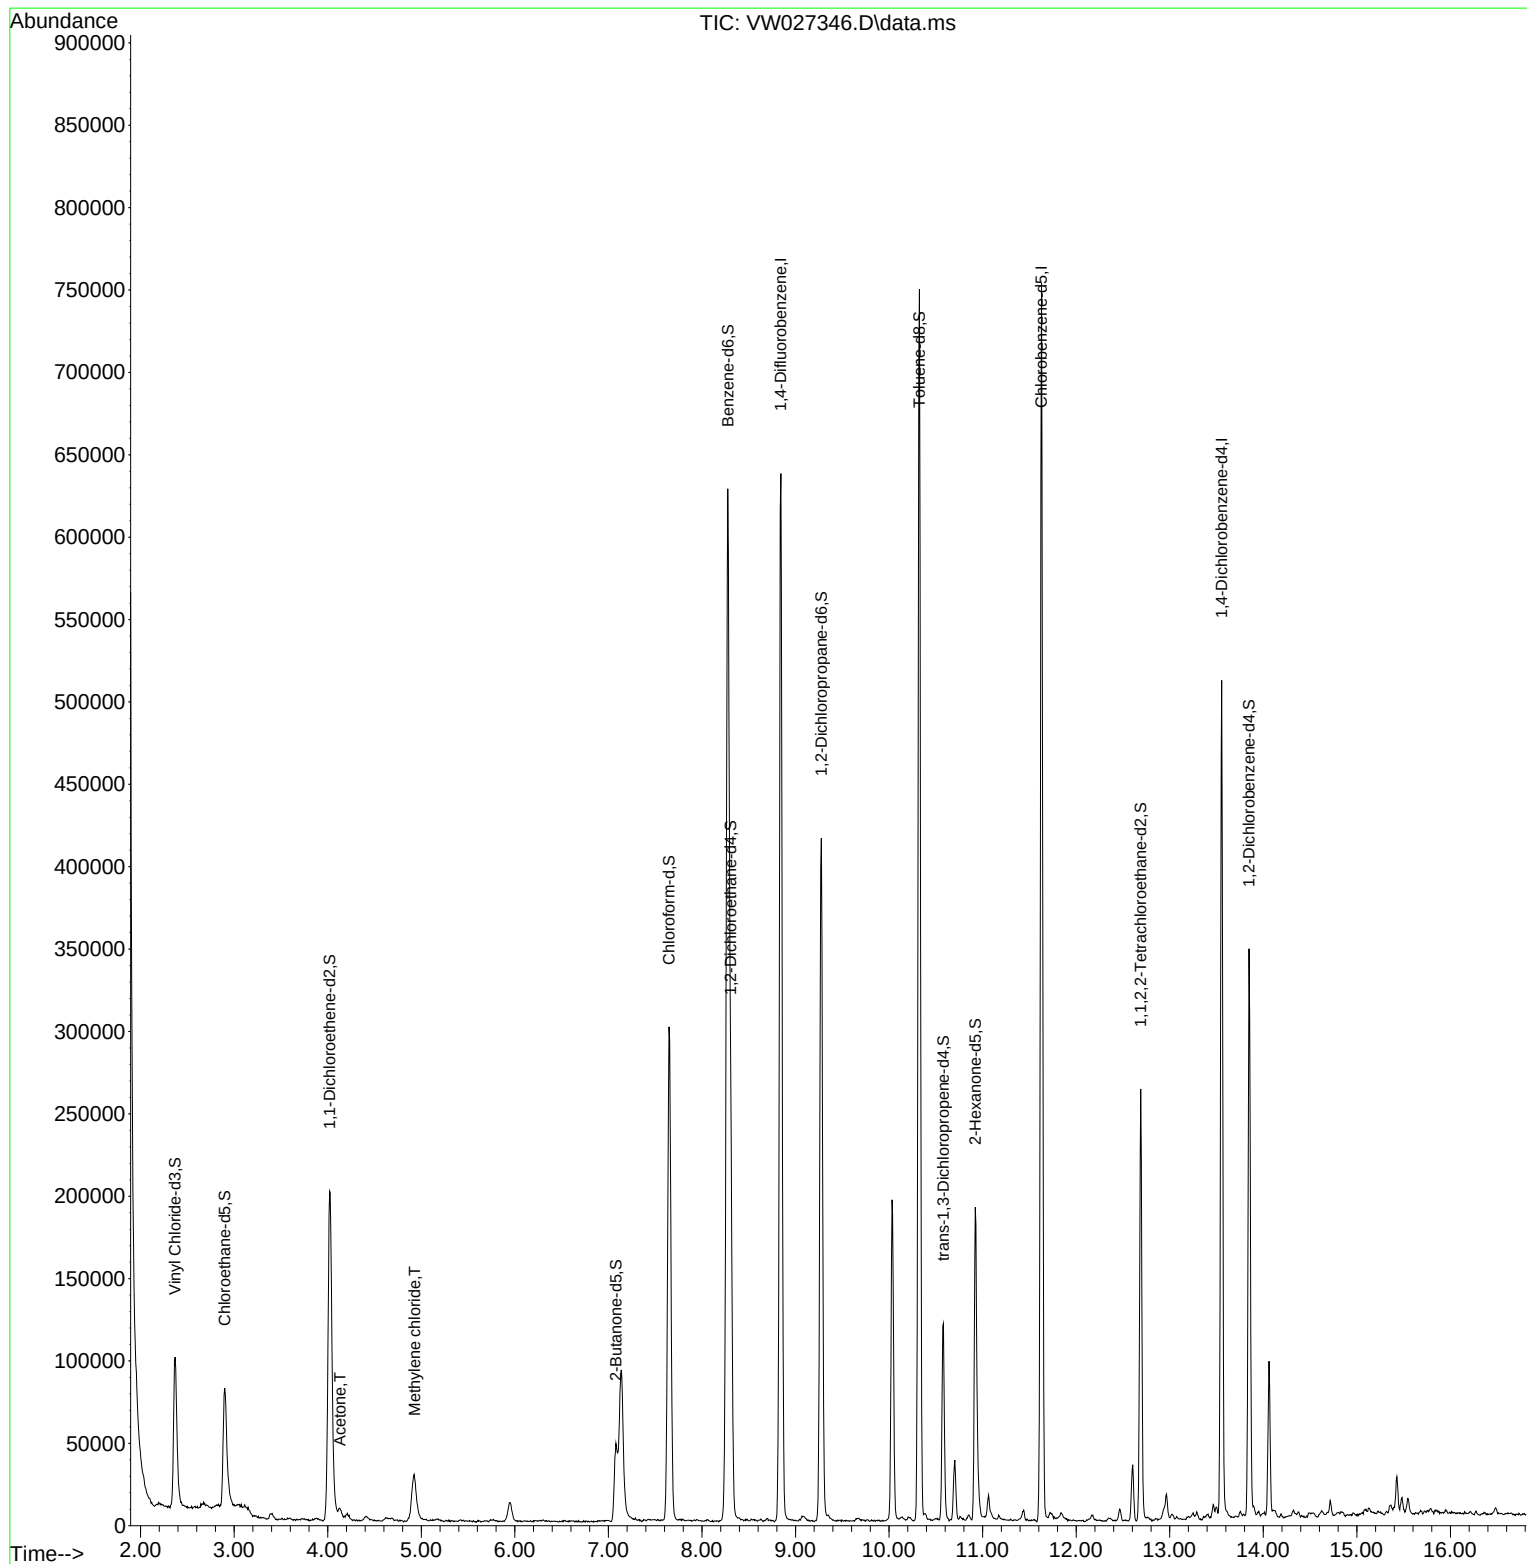

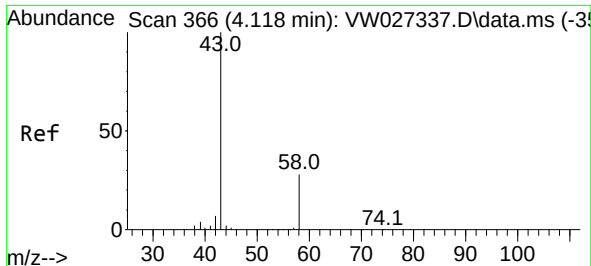





#13
Acetone
Concen: 4.576 ug/L
RT: 4.130 min Scan# 368
Delta R.T. 0.012 min
Lab File: VW027346.D
Acq: 19 Oct 2023 14:26

Instrument :
MSVOA_W
ClientSampleId :
EOAS0

Tgt Ion: 43 Resp: 1052
Ion Ratio Lower Upper
43 100
58 29.9 0.0 60.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/20/2023
Supervised By :Mahesh Dadoda 10/20/2023

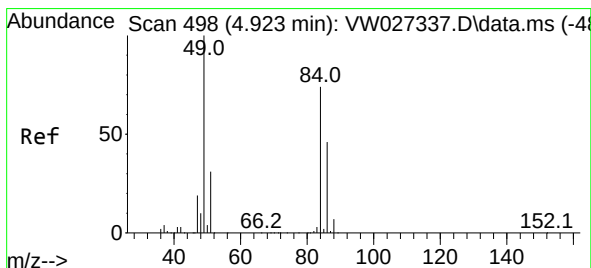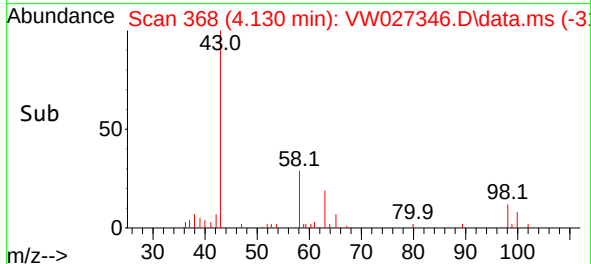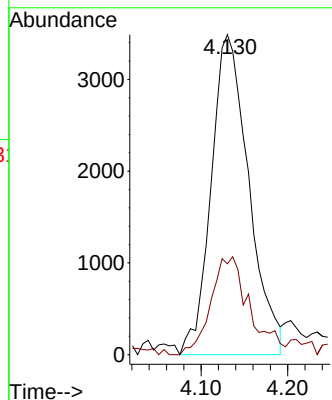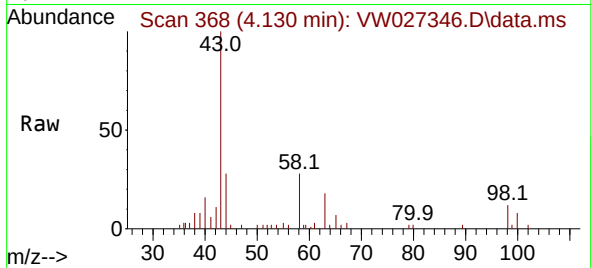

#16
Methylene chloride
Concen: 2.169 ug/L
RT: 4.929 min Scan# 499
Delta R.T. 0.006 min
Lab File: VW027346.D
Acq: 19 Oct 2023 14:26

Tgt Ion: 84 Resp: 20851
Ion Ratio Lower Upper
84 100
86 59.6 41.3 76.7
49 126.1 92.8 172.4

