




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
 Data File : VW027365.D
 Acq On : 20 Oct 2023 11:45
 Operator : SY/MD
 Sample : 04953-08
 Misc : 3.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAT5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 04:26:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 21 04:25:20 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/21/2023
 Supervised By :Mahesh Dadoda 10/24/2023

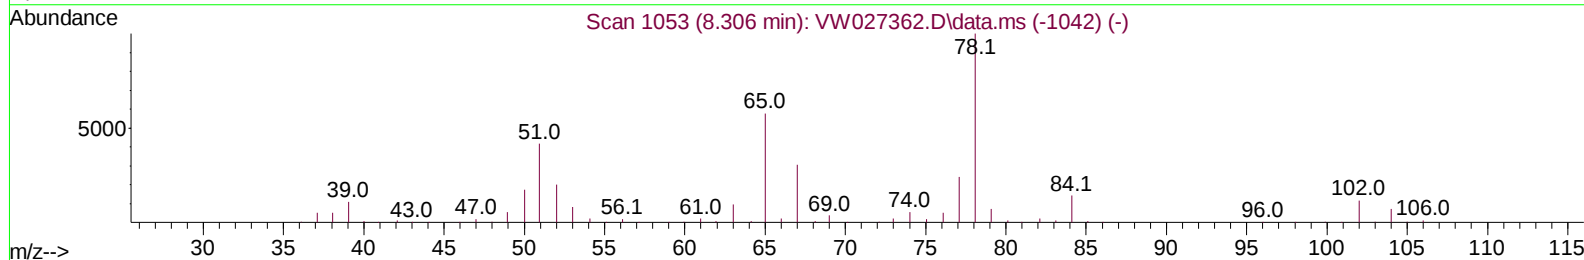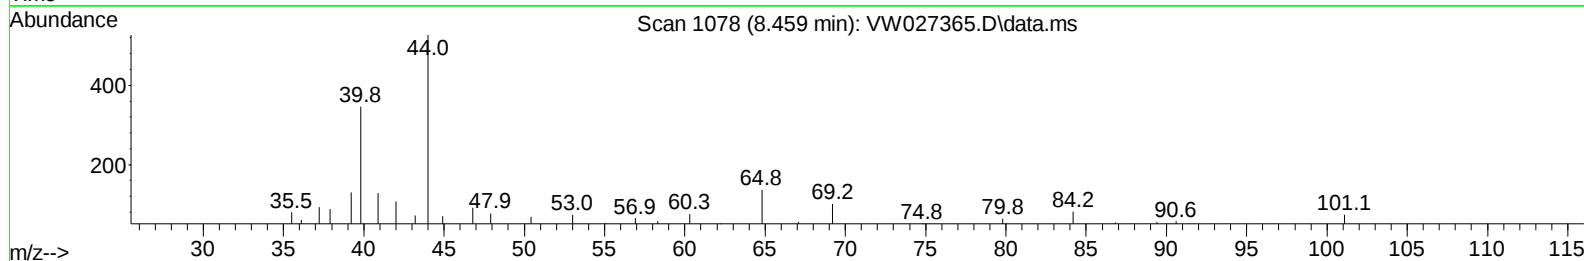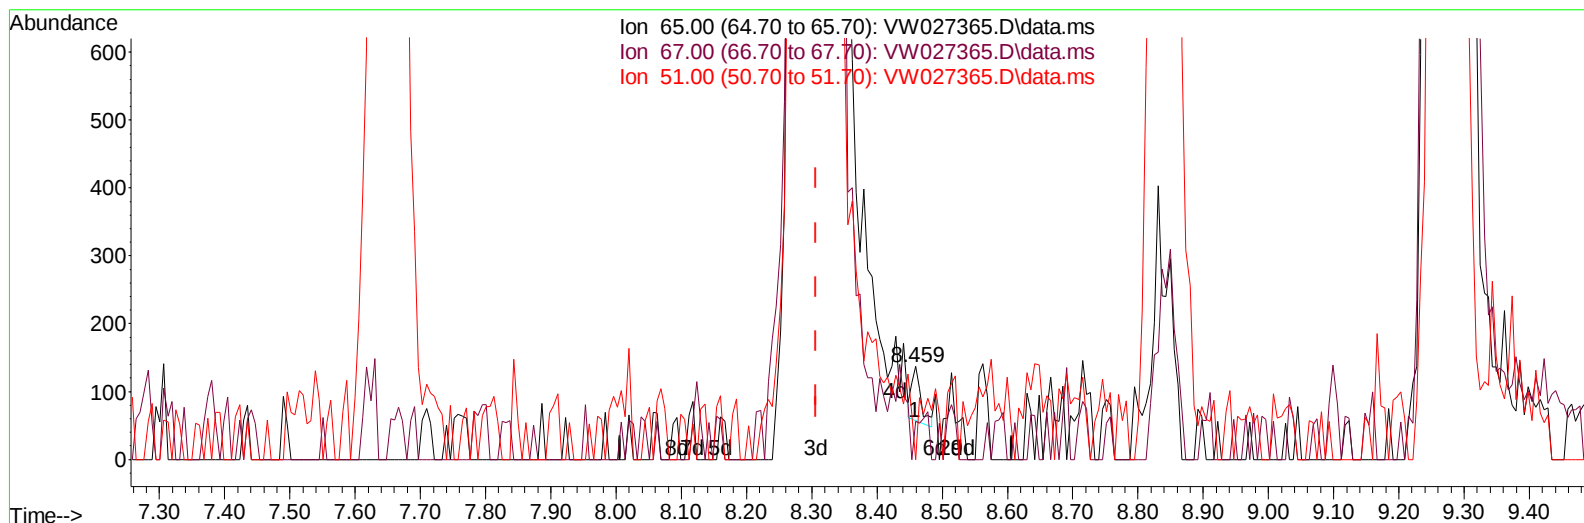

TIC: VW027365.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.459min (+ 0.153) 0.01 ug/L

response 78

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	51.28
51.00	99.60	74.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
 Data File : VW027365.D
 Acq On : 20 Oct 2023 11:45
 Operator : SY/MD
 Sample : 04953-08
 Misc : 3.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAT5

Manual IntegrationsAPPROVED

Quant Time: Oct 21 04:26:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 21 04:25:20 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/21/2023
 Supervised By :Mahesh Dadoda 10/24/2023

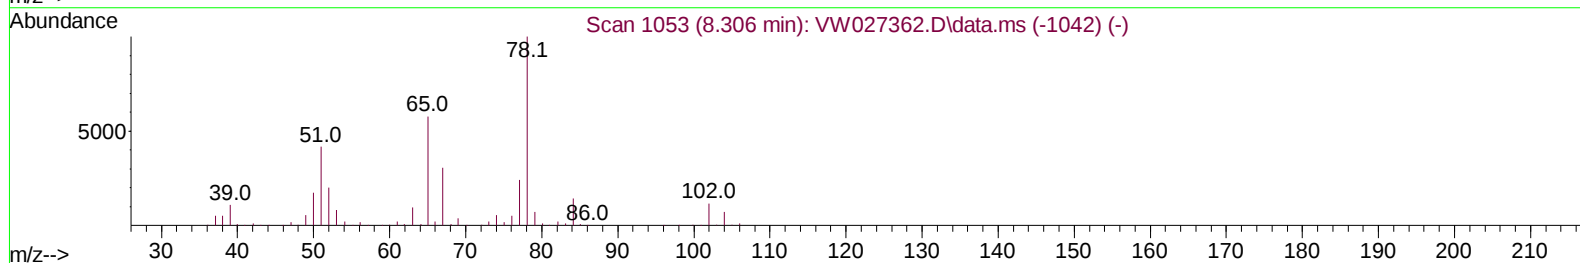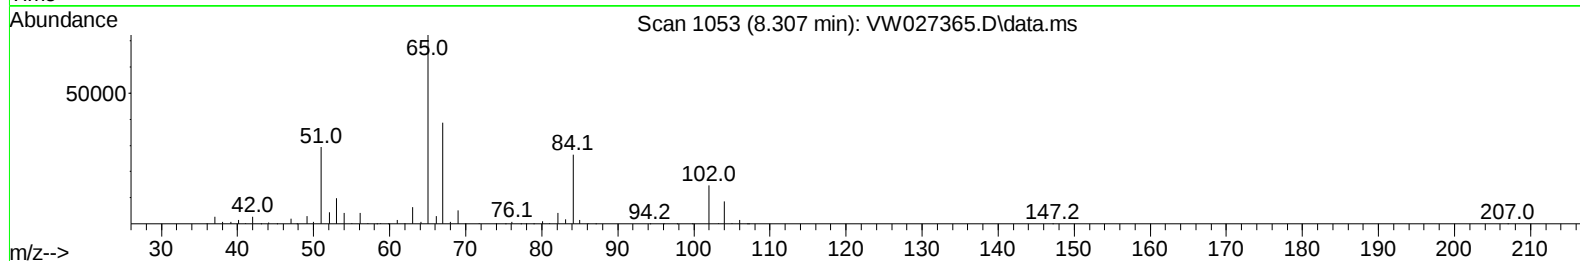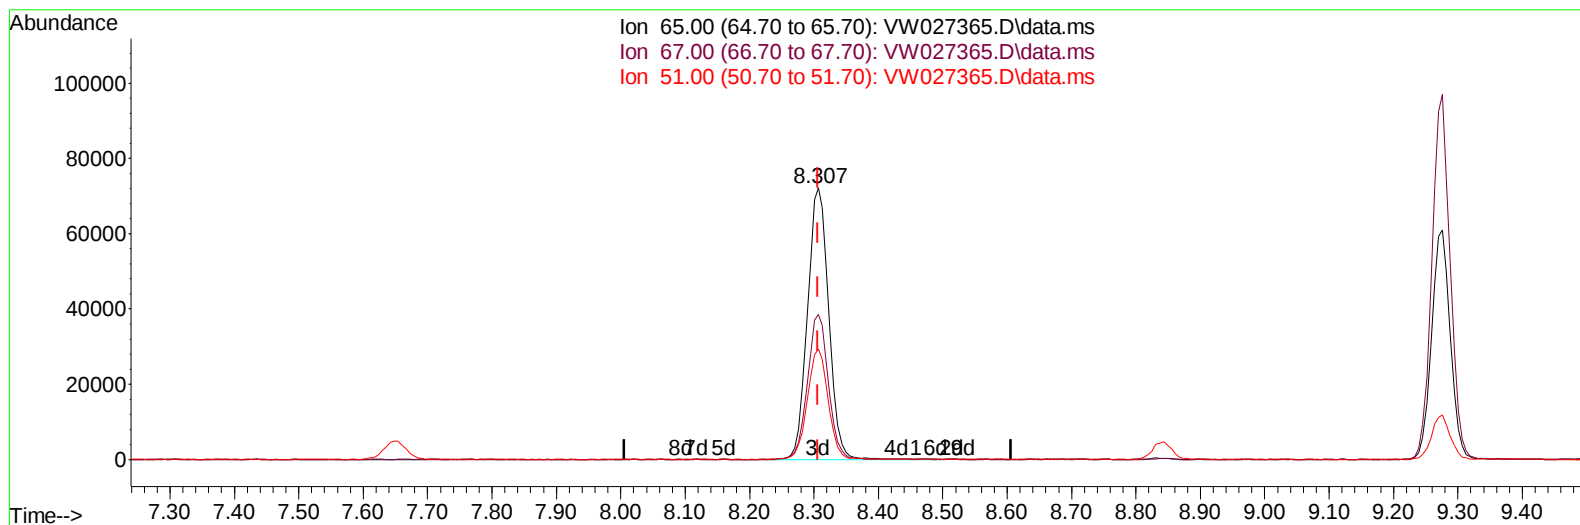

TIC: VW027365.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 23.38 ug/L m

response 165431

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.02#
51.00	99.60	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
 Data File : VW027365.D
 Acq On : 20 Oct 2023 11:45
 Operator : SY/MD
 Sample : 04953-08
 Misc : 3.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAT5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/21/2023
 Supervised By :Mahesh Dadoda 10/24/2023

Quant Time: Oct 21 04:26:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 21 04:25:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	441910	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	329034	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	101347	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	132344	19.623	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	78.480%		
7) Chloroethane-d5	2.893	69	105335	21.752	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	87.000%		
11) 1,1-Dichloroethene-d2	4.021	65	66414	19.653	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	78.600%		
21) 2-Butanone-d5	7.081	46	75744	33.790	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	67.580%		
24) Chloroform-d	7.648	84	291616	22.141	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	88.560%		
26) 1,2-Dichloroethane-d4	8.307	65	165431m	23.382	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	93.520%		
32) Benzene-d6	8.276	84	579699	26.040	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	104.160%		
36) 1,2-Dichloropropane-d6	9.276	67	191054	28.098	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	112.400%		
41) Toluene-d8	10.325	98	437546	21.674	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	86.680%		
43) trans-1,3-Dichloroprop...	10.575	79	62313	20.100	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	80.400%		
47) 2-Hexanone-d5	10.922	63	59316	42.164	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	84.320%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	122062	24.061	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	96.240%		
66) 1,2-Dichlorobenzene-d4	13.848	152	74197	20.203	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	80.800%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
Data File : VW027365.D
Acq On : 20 Oct 2023 11:45
Operator : SY/MD
Sample : 04953-08
Misc : 3.84g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAT5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/21/2023
Supervised By :Mahesh Dadoda 10/24/2023

Quant Time: Oct 21 04:26:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 21 04:25:20 2023
Response via : Initial Calibration

