

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
 Data File : VW027368.D
 Acq On : 20 Oct 2023 12:57
 Operator : SY/MD
 Sample : 04953-05
 Misc : 2.83g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAS7

Quant Time: Oct 21 04:28:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 21 04:25:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	493659	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	367596	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112058	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	124203	16.486	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.960%
7) Chloroethane-d5	2.893	69	102458	18.940	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.760%
11) 1,1-Dichloroethene-d2	4.021	65	64598	17.112	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.440%
21) 2-Butanone-d5	7.081	46	94183	37.611	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.220%
24) Chloroform-d	7.648	84	284547	19.339	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.360%
26) 1,2-Dichloroethane-d4	8.307	65	163650	20.705	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.840%
32) Benzene-d6	8.270	84	573806	23.072	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.280%
36) 1,2-Dichloropropane-d6	9.270	67	189148	24.900	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.600%
41) Toluene-d8	10.325	98	439299	19.478	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.920%
43) trans-1,3-Dichloroprop...	10.575	79	64524	18.630	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.520%
47) 2-Hexanone-d5	10.922	63	74458	47.375	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.760%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	137282	24.222	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	78478	19.326	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.320%
Target Compounds					Qvalue	
13) Acetone	4.143	43	15206	7.031	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
Data File : VW027368.D
Acq On : 20 Oct 2023 12:57
Operator : SY/MD
Sample : 04953-05
Misc : 2.83g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAS7

Quant Time: Oct 21 04:28:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 21 04:25:20 2023
Response via : Initial Calibration

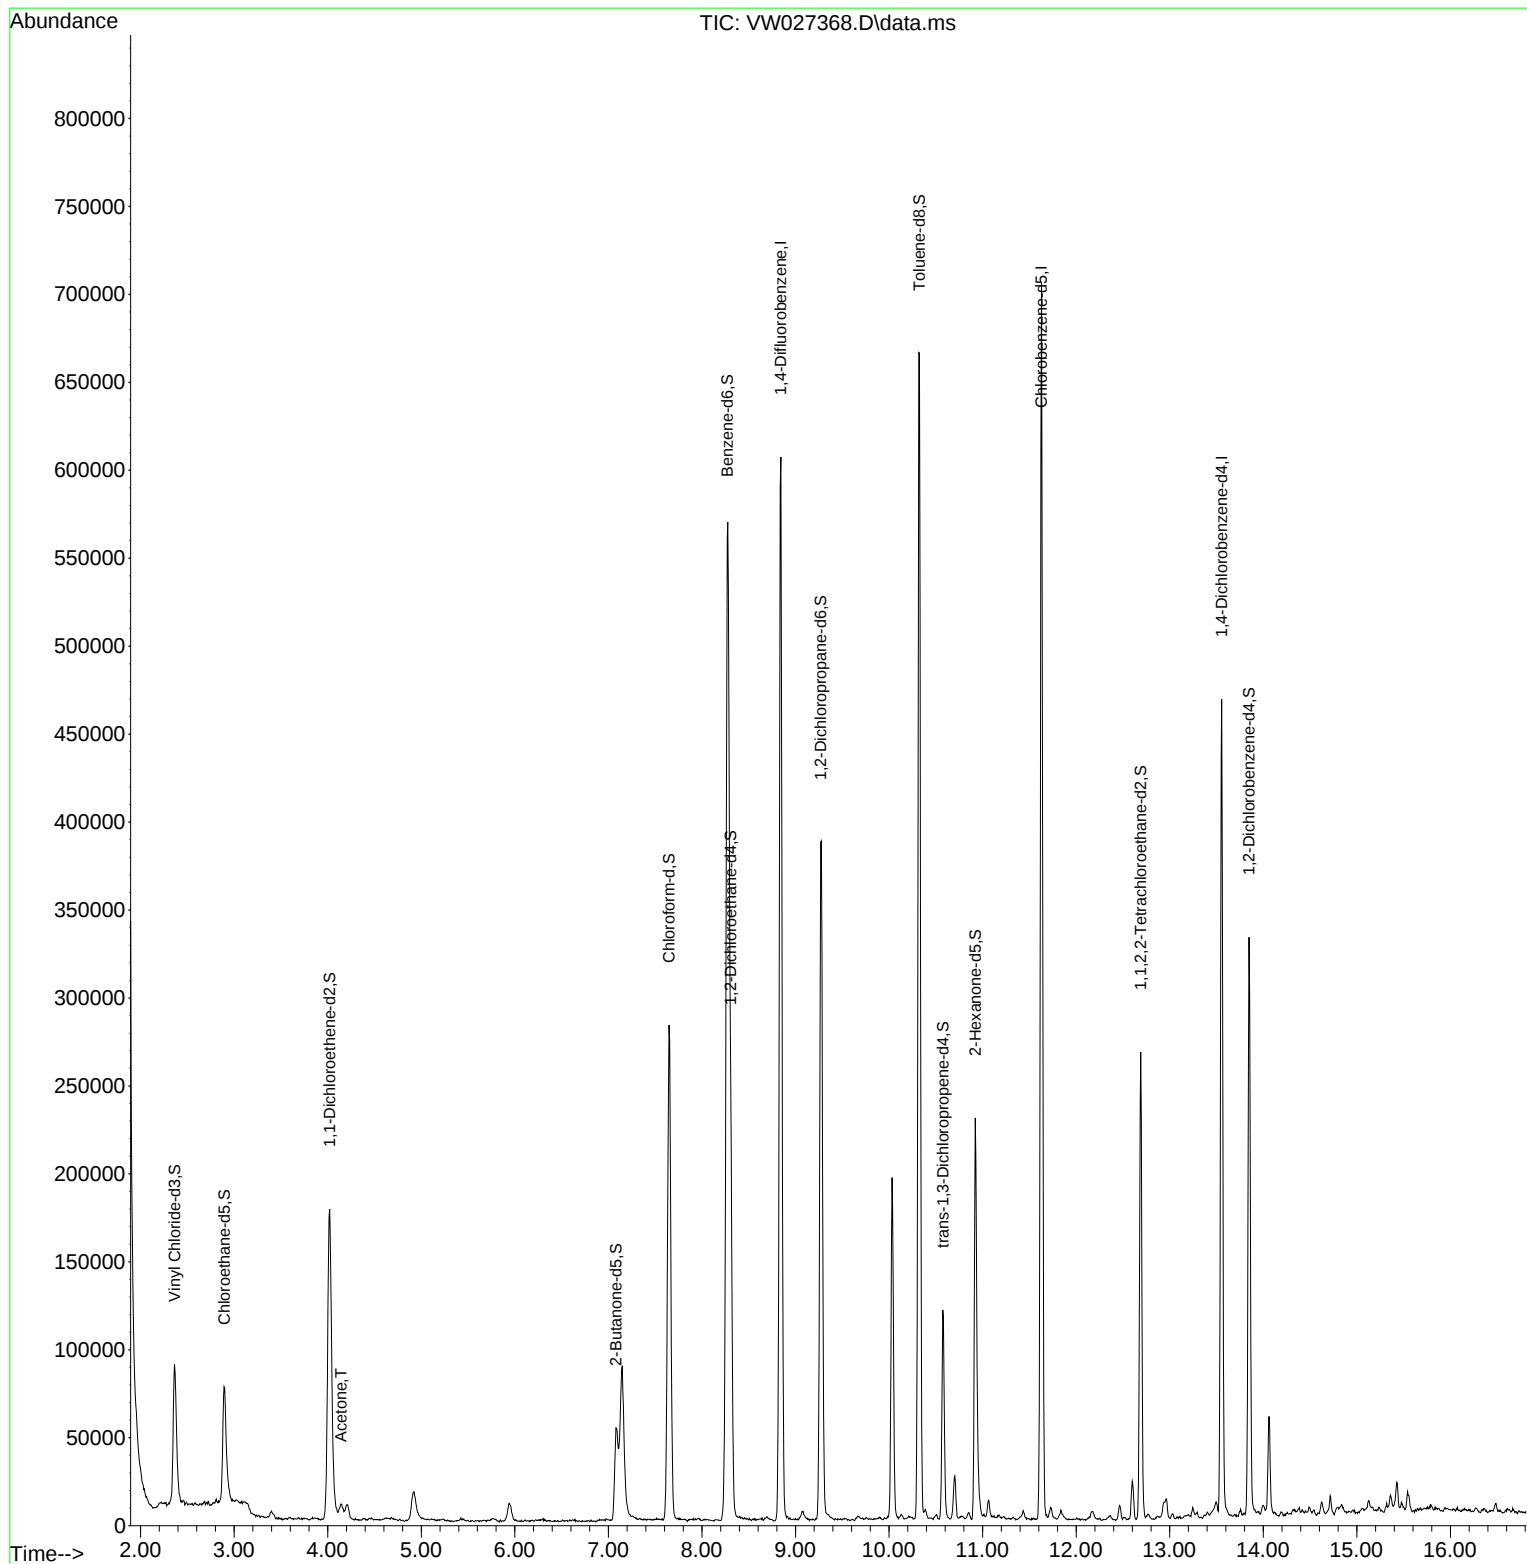

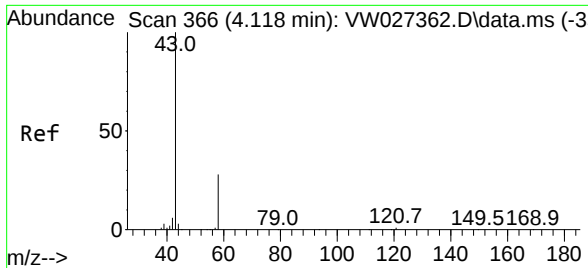

#13
 Acetone
 Concen: 7.031 ug/L
 RT: 4.143 min Scan# 31
 Delta R.T. 0.025 min
 Lab File: VW027368.D
 Acq: 20 Oct 2023 12:57

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAS7

Tgt Ion: 43 Resp: 15206
 Ion Ratio Lower Upper
 43 100
 58 30.8 0.0 60.8

