

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
 Data File : VW027369.D
 Acq On : 20 Oct 2023 13:21
 Operator : SY/MD
 Sample : 04953-07RE
 Misc : 3.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAS9RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/21/2023
 Supervised By :Mahesh Dadoda 10/24/2023

Quant Time: Oct 21 04:28:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 21 04:25:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	430773	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	308023	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	90695	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	124793	18.982	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.920%		
7) Chloroethane-d5	2.899	69	100477	21.285	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.160%		
11) 1,1-Dichloroethene-d2	4.021	65	60418	18.341	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.360%		
21) 2-Butanone-d5	7.075	46	106372	48.680	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.360%		
24) Chloroform-d	7.648	84	269296	20.975	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.880%		
26) 1,2-Dichloroethane-d4	8.307	65	156577m	22.703	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.800%		
32) Benzene-d6	8.276	84	542889	26.050	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	104.200%		
36) 1,2-Dichloropropane-d6	9.276	67	178217	27.998	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	112.000%		
41) Toluene-d8	10.325	98	399520	21.141	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.560%		
43) trans-1,3-Dichloroprop...	10.575	79	57028	19.650	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.600%		
47) 2-Hexanone-d5	10.922	63	76886	58.382	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	116.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	126975	26.737	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	106.960%		
66) 1,2-Dichlorobenzene-d4	13.848	152	66797	20.324	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.280%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	35352	18.731	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102023\
Data File : VW027369.D
Acq On : 20 Oct 2023 13:21
Operator : SY/MD
Sample : 04953-07RE
Misc : 3.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAS9RE

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 10/21/2023
Supervised By : Mahesh Dadoda 10/24/2023


Quant Time: Oct 21 04:28:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 21 04:25:20 2023
Response via : Initial Calibration

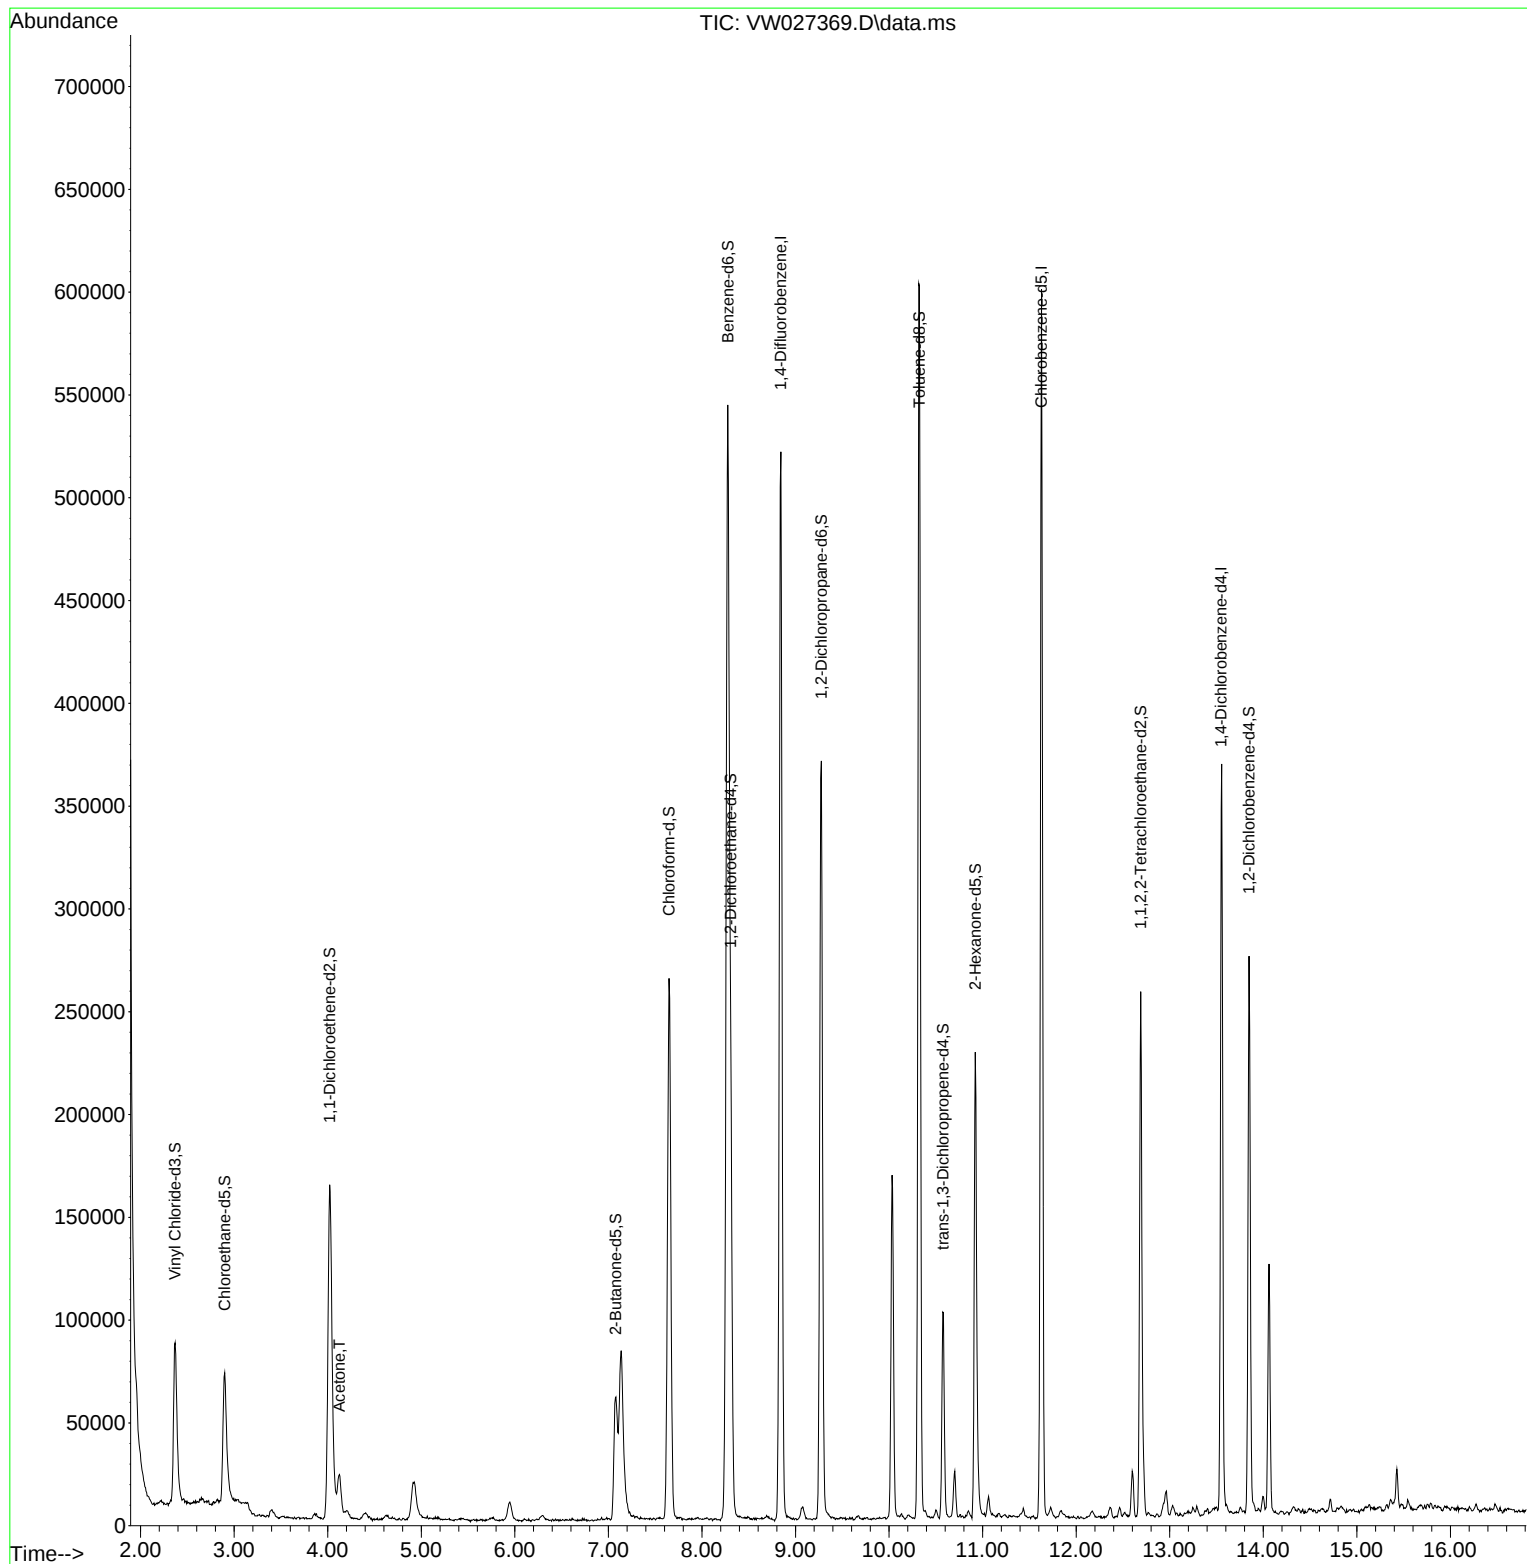

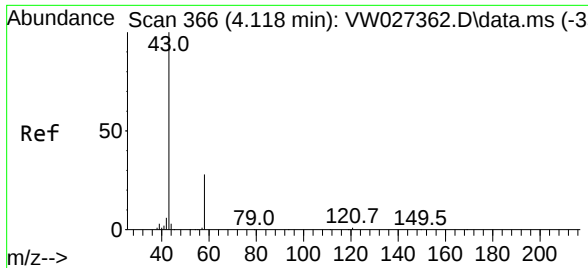

#13
 Acetone
 Concen: 18.731 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.007 min
 Lab File: VW027369.D
 Acq: 20 Oct 2023 13:21

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAS9RE

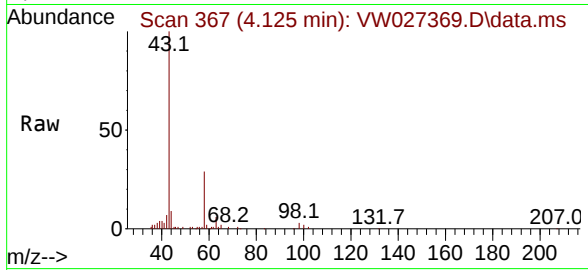

Tgt Ion: 43 Resp: 35352
 Ion Ratio Lower Upper
 43 100
 58 31.0 0.0 60.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/21/2023
 Supervised By :Mahesh Dadoda 10/24/2023

