

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102025\
 Data File : VW032399.D
 Acq On : 20 Oct 2025 18:58
 Operator : SY/MD
 Sample : Q3395-07
 Misc : 4.56g/5mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 PR132-S08-038048-20251017

Quant Time: Oct 21 01:34:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 02 21:24:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.959	168	239838	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	525260	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	508147	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	246462	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	203068	58.050	ug/l	0.00
Spiked Amount 50.000	Range 63 - 155		Recovery = 116.100%			
35) Dibromofluoromethane	7.904	113	174150	51.196	ug/l	0.00
Spiked Amount 50.000	Range 70 - 134		Recovery = 102.400%			
50) Toluene-d8	10.331	98	634729	50.557	ug/l	0.00
Spiked Amount 50.000	Range 74 - 123		Recovery = 101.120%			
62) 4-Bromofluorobenzene	12.617	95	307677	64.839	ug/l	0.00
Spiked Amount 50.000	Range 17 - 146		Recovery = 129.680%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.234	59	2145	8.101	ug/l #	69
13) Acrolein	3.929	56	2042	4.752	ug/l #	14
16) Acetone	4.161	43	188988	195.110	ug/l	100
17) Carbon Disulfide	4.417	76	28260	3.832	ug/l #	94
18) Methyl Acetate	4.716	43	8634	3.112	ug/l	98
20) Methylene Chloride	4.960	84	15634	Below Cal		91
25) 2-Butanone	7.197	43	77218	58.533	ug/l	99
31) Cyclohexane	7.959	56	8774	1.782	ug/l #	28
36) 1,1-Dichloropropene	7.959	75	19919	4.149	ug/l #	52
37) Ethyl Acetate	7.197	43	77218	24.165	ug/l #	69
38) Carbon Tetrachloride	7.965	117	27671	6.125	ug/l #	17
39) Methylcyclohexane	9.307	83	35554	6.140	ug/l #	27
43) Isopropyl Acetate	8.435	43	12839	2.265	ug/l #	52
47) Bromodichloromethane	9.617	83	11395	2.157	ug/l #	42
48) Methyl methacrylate	9.471	41	3015	1.094	ug/l #	9
51) 4-Methyl-2-Pentanone	10.215	43	6375	1.942	ug/l #	35
55) 1,1,2-Trichloroethane	10.764	97	26915	8.719	ug/l #	22
56) Ethyl methacrylate	10.623	69	195385	45.222	ug/l #	72
59) 2-Hexanone	10.934	43	138745	59.917	ug/l #	30
71) Bromoform	12.282	173	9310	4.664	ug/l #	36
73) Isopropylbenzene	12.465	105	23774	1.410	ug/l	94
74) N-amyl acetate	12.245	43	347663	64.631	ug/l #	42
75) 1,1,2,2-Tetrachloroethane	12.684	83	36836	8.798	ug/l #	25
76) 1,2,3-Trichloropropane	12.617	75	122041	37.628	ug/l #	1
77) Bromobenzene	12.843	156	60015	14.765	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.617	75	122041	95.323	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.251	105	17571	1.185	ug/l	79
92) 1,2-Dibromo-3-Chloropr...	14.263	75	822	1.121	ug/l	95
95) Naphthalene	15.360	128	10910	1.018	ug/l #	74
96) 1,2,3-Trichlorobenzene	15.513	180	8242	1.960	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102025\
Data File : VW032399.D
Acq On : 20 Oct 2025 18:58
Operator : SY/MD
Sample : Q3395-07
Misc : 4.56g/5mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017

Quant Time: Oct 21 01:34:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 02 21:24:16 2025
Response via : Initial Calibration




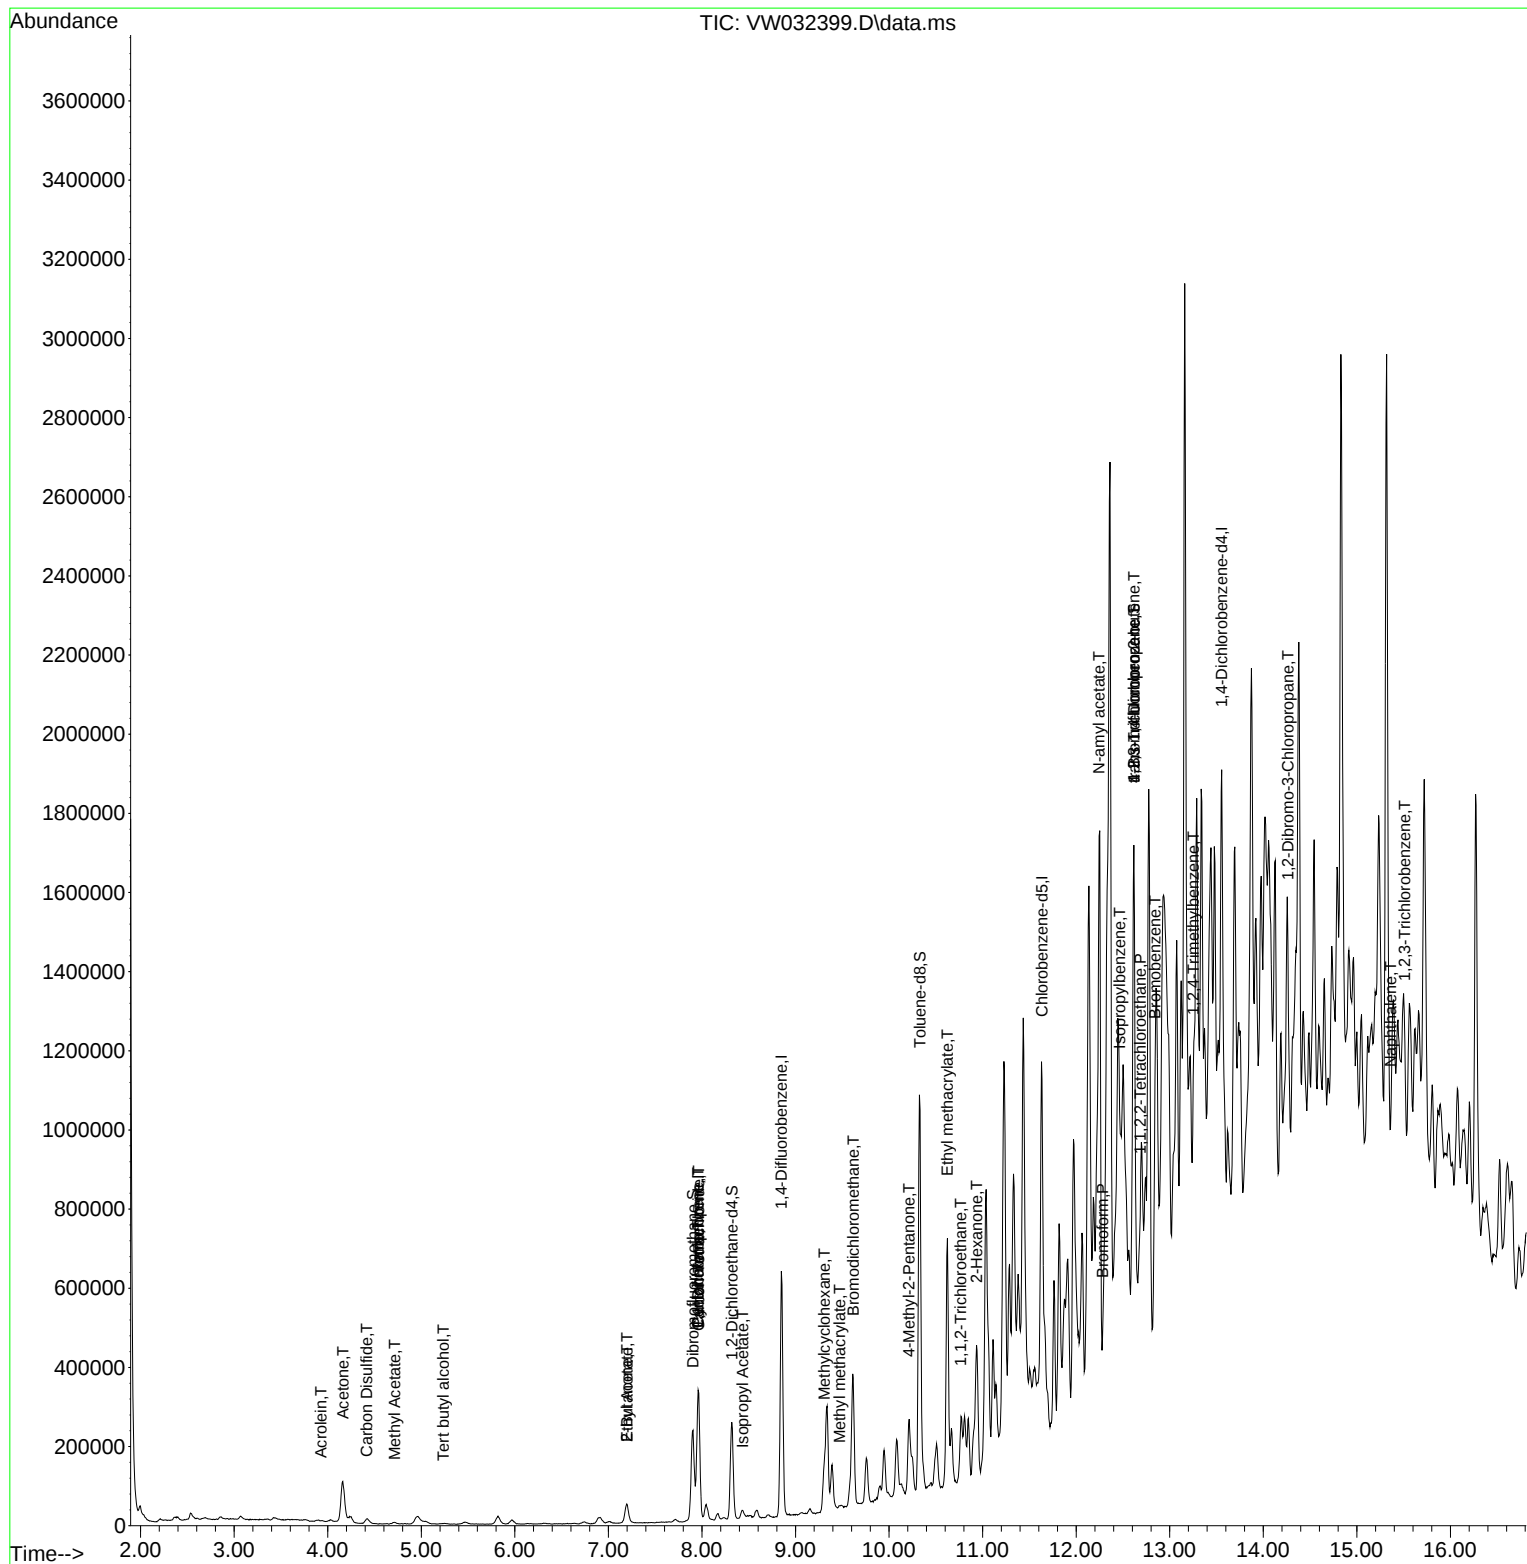




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion:168 Resp: 239838
Ion Ratio Lower Upper
168 100
99 63.1 49.3 73.9

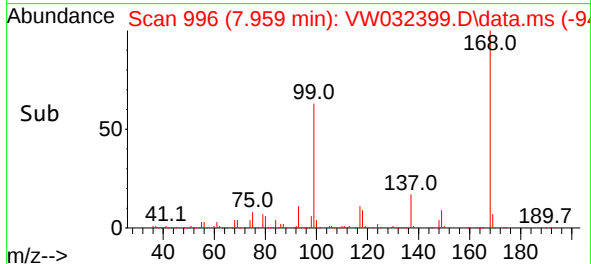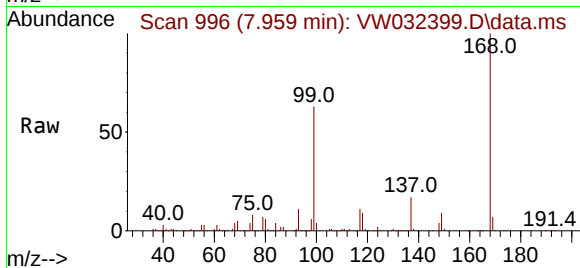

#11
Tert butyl alcohol
Concen: 8.101 ug/l
RT: 5.234 min Scan# 549
Delta R.T. 0.012 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 59 Resp: 2145
Ion Ratio Lower Upper
59 100
57 0.0 9.8 14.6#




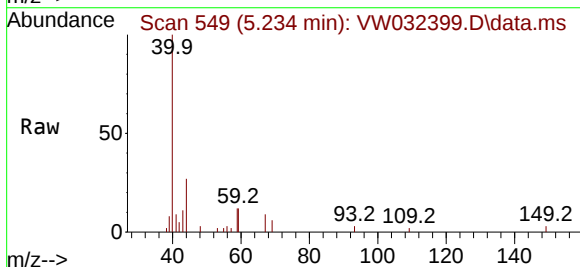


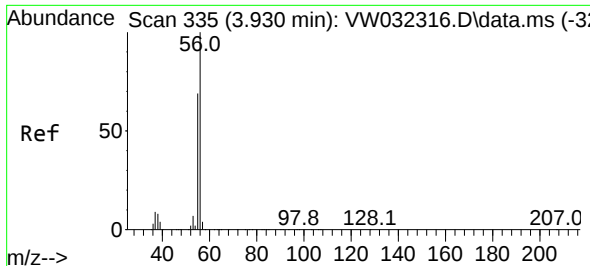

#13
Acrolein
Concen: 4.752 ug/l
RT: 3.929 min Scan# 31
Delta R.T. -0.000 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 56 Resp: 2042
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#

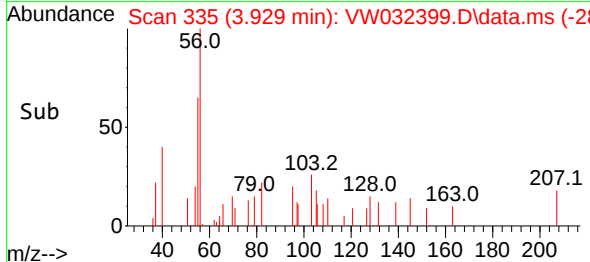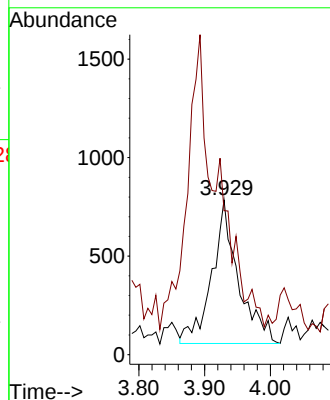

#16
Acetone
Concen: 195.110 ug/l
RT: 4.161 min Scan# 373
Delta R.T. -0.000 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 43 Resp: 188988
Ion Ratio Lower Upper
43 100
58 31.8 25.3 37.9


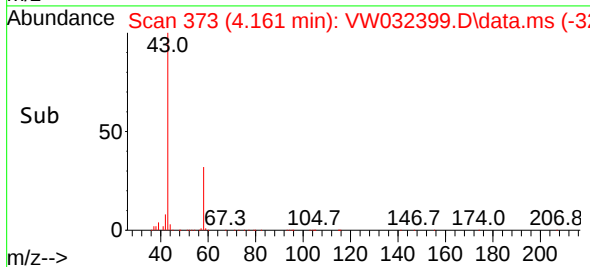
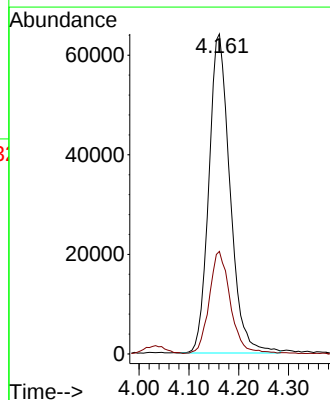
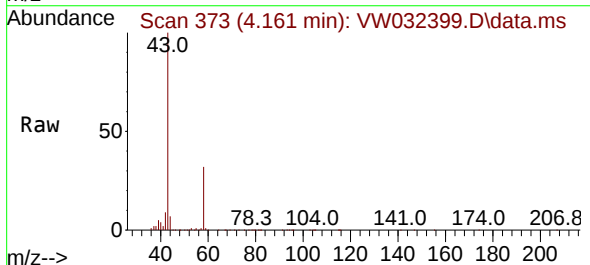




#17
Carbon Disulfide
Concen: 3.832 ug/l
RT: 4.417 min Scan# 416
Delta R.T. -0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 76 Resp: 28260
Ion Ratio Lower Upper
76 100
78 10.9 7.0 10.6#

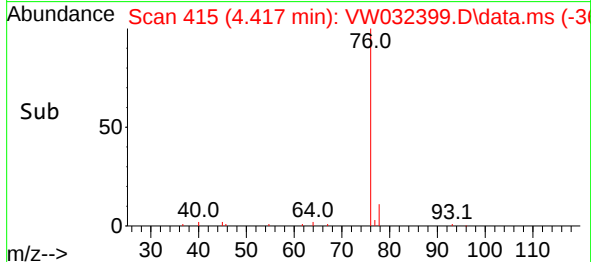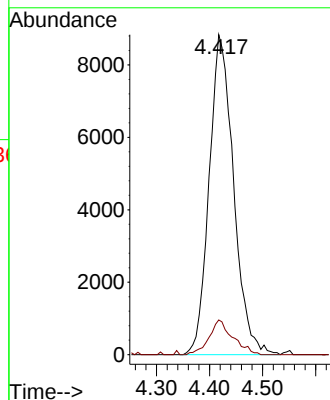

#18
Methyl Acetate
Concen: 3.112 ug/l
RT: 4.716 min Scan# 464
Delta R.T. 0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 43 Resp: 8634
Ion Ratio Lower Upper
43 100
74 24.1 20.2 30.4



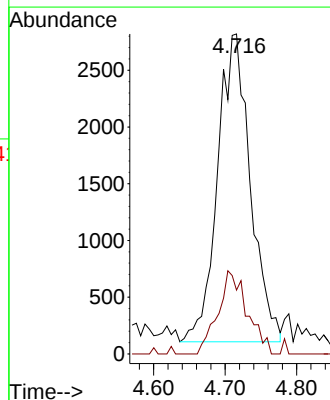
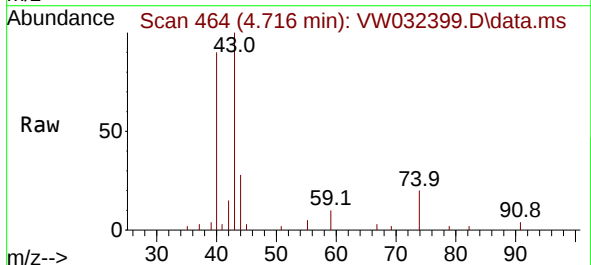




#25
2-Butanone
Concen: 58.533 ug/l
RT: 7.197 min Scan# 81
Delta R.T. 0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 43 Resp: 77218
Ion Ratio Lower Upper
43 100
72 26.2 21.4 32.2

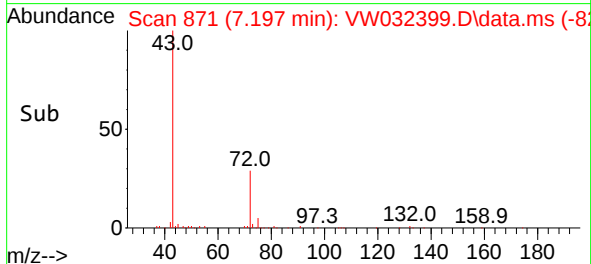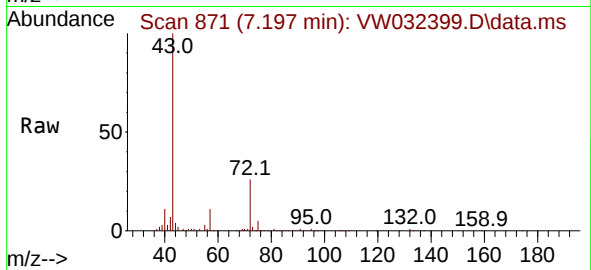

#31
Cyclohexane
Concen: 1.782 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.012 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 56 Resp: 8774
Ion Ratio Lower Upper
56 100
69 131.3 27.7 41.5#
84 128.8 74.6 112.0#


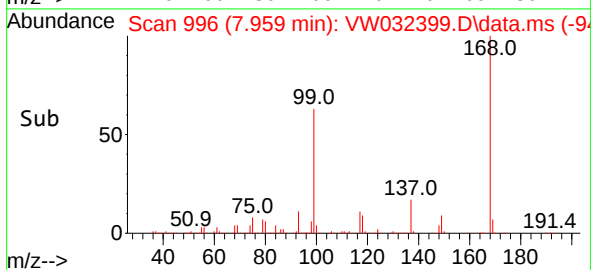




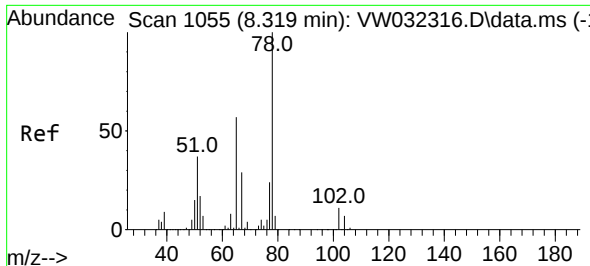

#33
 1,2-Dichloroethane-d4
 Concen: 58.050 ug/l
 RT: 8.319 min Scan# 1105
 Delta R.T. -0.000 min
 Lab File: VW032399.D
 Acq: 20 Oct 2025 18:58




Instrument :
 MSVOA_W
 ClientSampleId :
 PR132-S08-038048-20251017


Tgt Ion: 65 Resp: 203068
 Ion Ratio Lower Upper
 65 100
 67 50.6 0.0 99.6

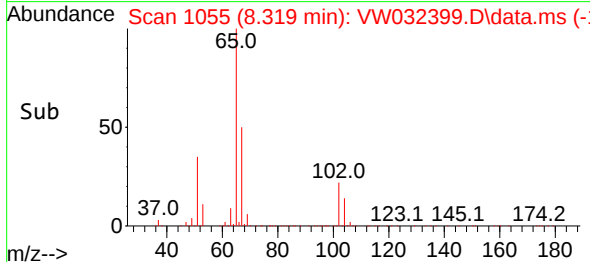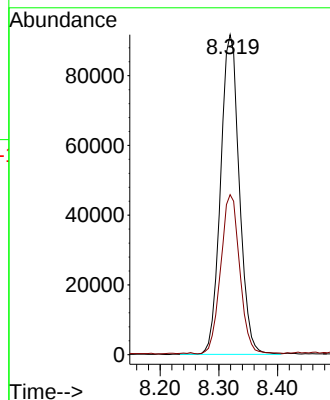

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.849 min Scan# 1142
 Delta R.T. -0.006 min
 Lab File: VW032399.D
 Acq: 20 Oct 2025 18:58

Tgt Ion: 114 Resp: 525260
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 40.4
 88 15.9 0.0 32.0


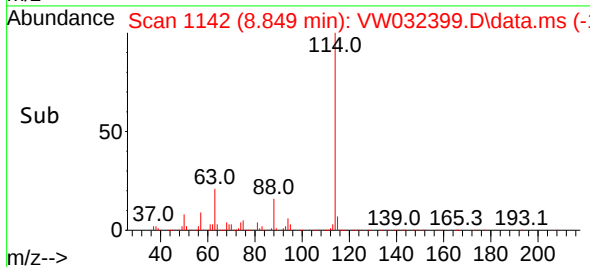
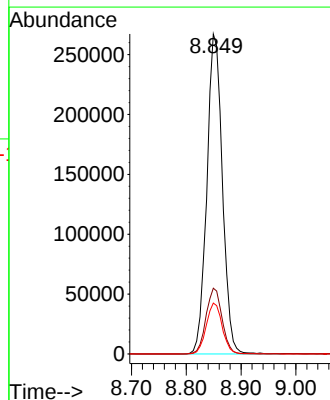
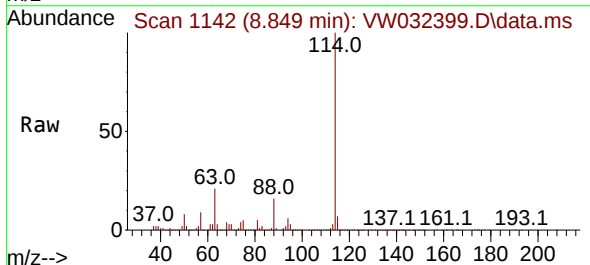


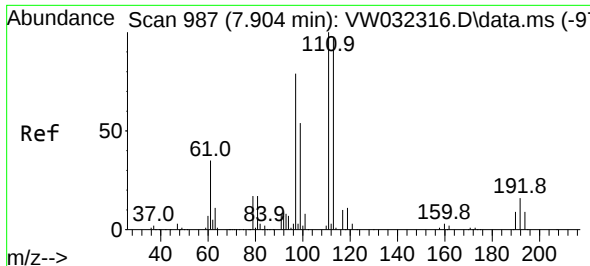

#35
Dibromofluoromethane
Concen: 51.196 ug/l
RT: 7.904 min Scan# 911
Delta R.T. -0.000 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion:113 Resp: 174150
Ion Ratio Lower Upper
113 100
111 102.6 83.9 125.9
192 16.0 14.6 21.8

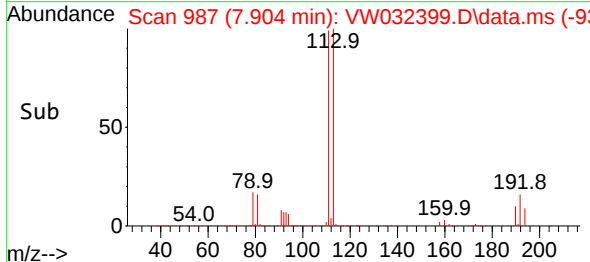

#36
1,1-Dichloropropene
Concen: 4.149 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.140 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 75 Resp: 19919
Ion Ratio Lower Upper
75 100
110 9.7 17.5 52.5#
77 1.1 24.1 36.1#

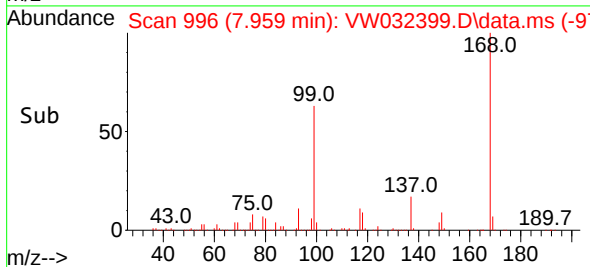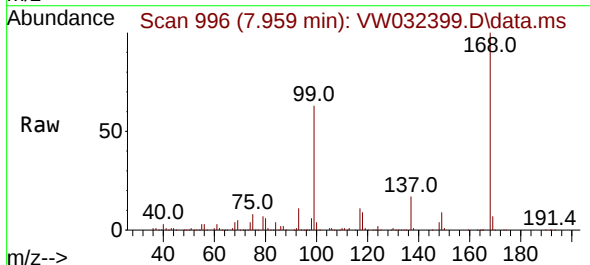

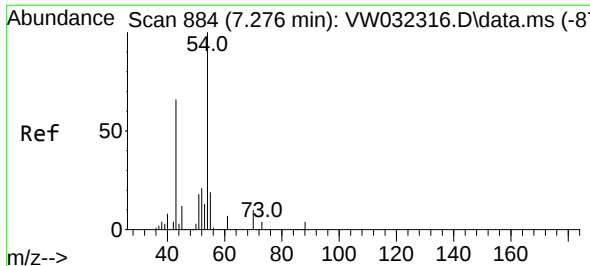

#37

Ethyl Acetate

Concen: 24.165 ug/l

RT: 7.197 min Scan# 81

Delta R.T. -0.079 min

Lab File: VW032399.D


Acq: 20 Oct 2025 18:58

Instrument :

MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017






Tgt Ion: 43 Resp: 77218

Ion Ratio Lower Upper

43 100

61 0.0 11.3 16.9#

70 0.7 8.9 13.3#

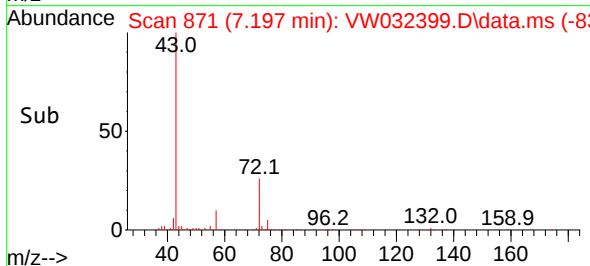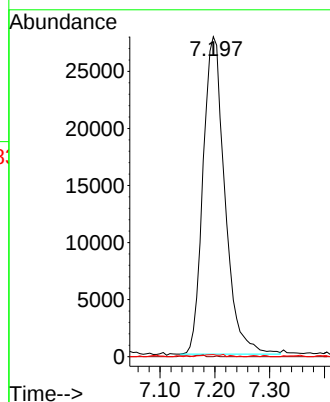

#38

Carbon Tetrachloride

Concen: 6.125 ug/l

RT: 7.965 min Scan# 997

Delta R.T. -0.122 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58




Tgt Ion: 117 Resp: 27671


Ion Ratio Lower Upper

117 100

119 4.6 74.2 111.2#

121 0.0 25.6 38.4#

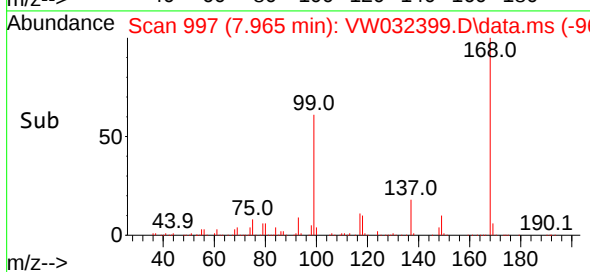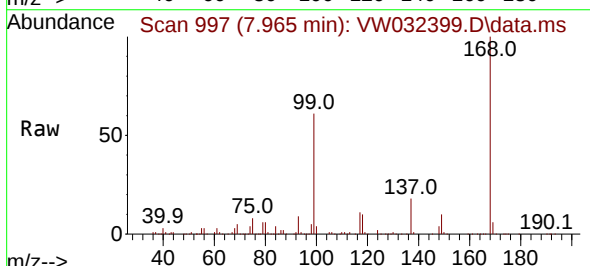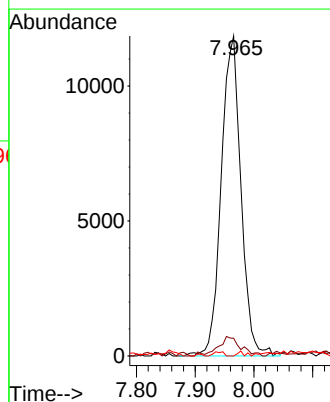

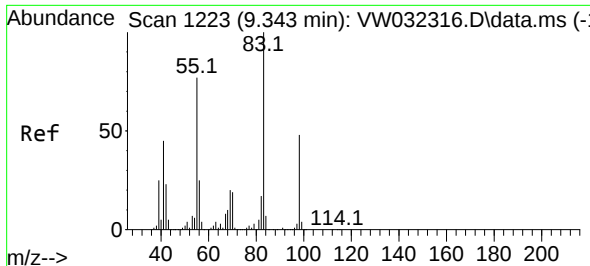

#39

Methylcyclohexane

Concen: 6.140 ug/l

RT: 9.307 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Instrument :





MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017

Tgt Ion: 83 Resp: 35554

Ion	Ratio	Lower	Upper
83	100		
55	142.6	58.4	87.6#
98	9.5	39.4	59.2#

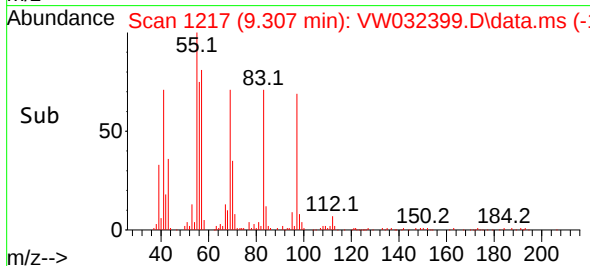

#43

Isopropyl Acetate

Concen: 2.265 ug/l

RT: 8.435 min Scan# 1074




Delta R.T. -0.000 min


Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Tgt Ion: 43 Resp: 12839

Ion	Ratio	Lower	Upper
43	100		
61	0.0	23.3	34.9#
87	0.0	11.1	16.7#

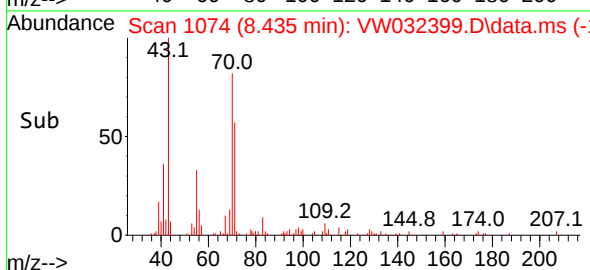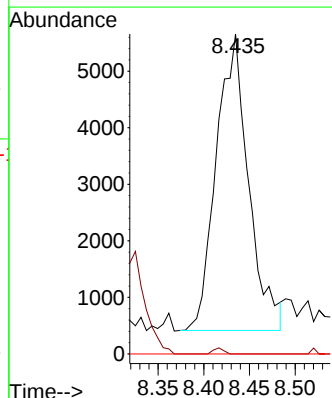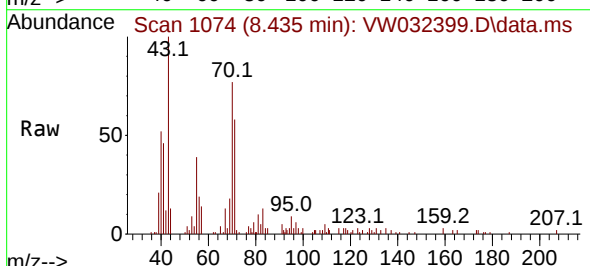



#47

Bromodichloromethane

Concen: 2.157 ug/l

RT: 9.617 min Scan# 11

Delta R.T. -0.031 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Instrument :

MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017





Tgt Ion: 83 Resp: 11395

Ion Ratio Lower Upper

83 100

85 13.2 48.7 73.1#

127 0.0 6.4 9.6#

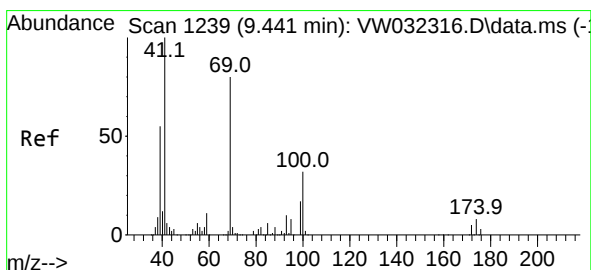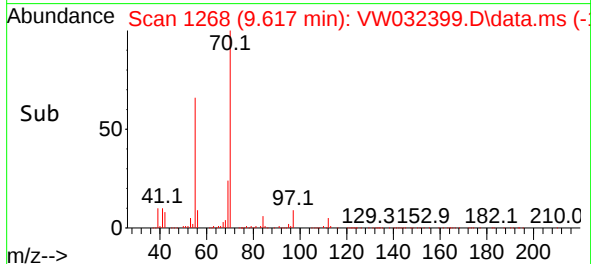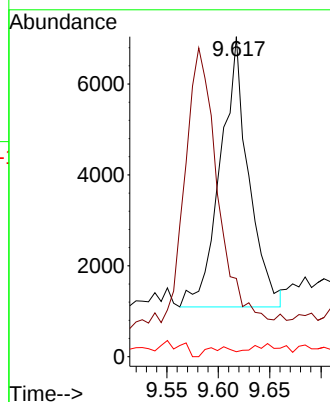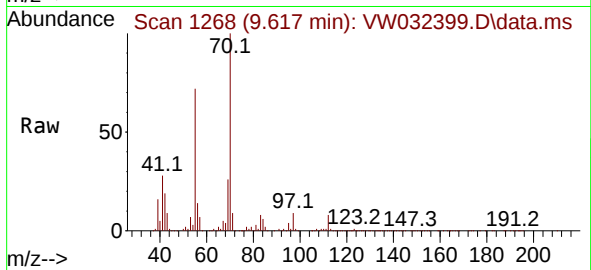

#48

Methyl methacrylate

Concen: 1.094 ug/l

RT: 9.471 min Scan# 1244

Delta R.T. 0.030 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58




Tgt Ion: 41 Resp: 3015


Ion Ratio Lower Upper

41 100

69 0.0 71.5 107.3#

39 0.0 55.9 83.9#



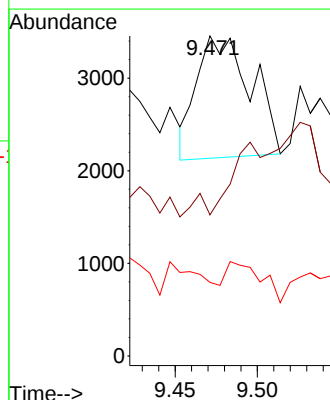





#50
Toluene-d8
Concen: 50.557 ug/l
RT: 10.331 min Scan# 1385
Delta R.T. 0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 98 Resp: 634729
Ion Ratio Lower Upper
98 100
100 66.2 51.4 77.2

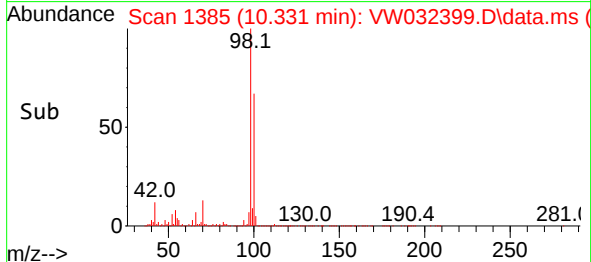

#51
4-Methyl-2-Pentanone
Concen: 1.942 ug/l
RT: 10.215 min Scan# 1366
Delta R.T. -0.000 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 43 Resp: 6375
Ion Ratio Lower Upper
43 100
58 0.0 32.0 48.0#




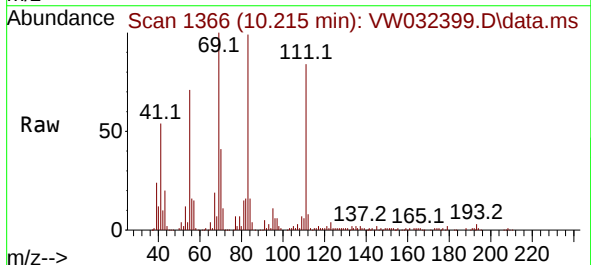




#55
1,1,2-Trichloroethane
Concen: 8.719 ug/l
RT: 10.764 min Scan# 1456
Delta R.T. -0.024 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument : MSVOA_W
ClientSampleId : PR132-S08-038048-20251017


Tgt Ion: 97	Resp: 26915
Ion Ratio	Lower Upper
97	100
83	13.1 71.0 106.6#
85	103.3 42.8 64.2#
99	0.0 51.0 76.6#

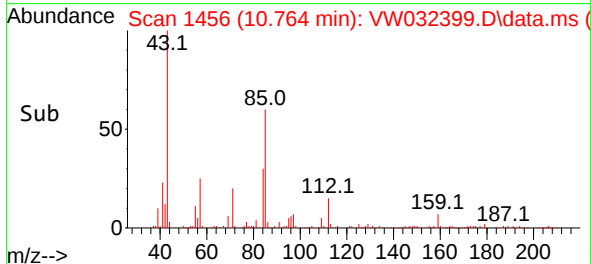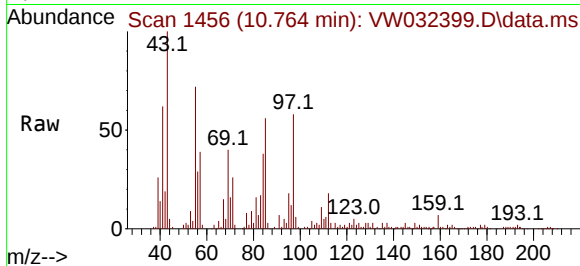

#56
Ethyl methacrylate
Concen: 45.222 ug/l
RT: 10.623 min Scan# 1433
Delta R.T. -0.024 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 69	Resp: 195385
Ion Ratio	Lower Upper
69	100
41	47.0 53.2 79.8#
39	19.8 32.9 49.3#


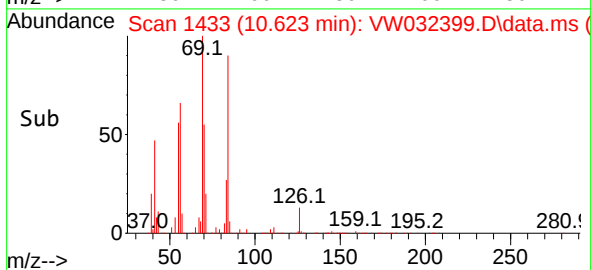

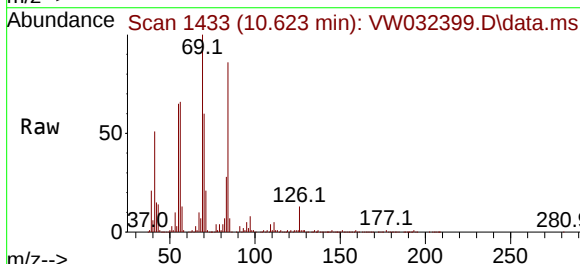




#59
2-Hexanone
Concen: 59.917 ug/l
RT: 10.934 min Scan# 1490
Delta R.T. -0.037 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 43 Resp: 138745
Ion Ratio Lower Upper
43 100
58 4.7 27.5 82.4#

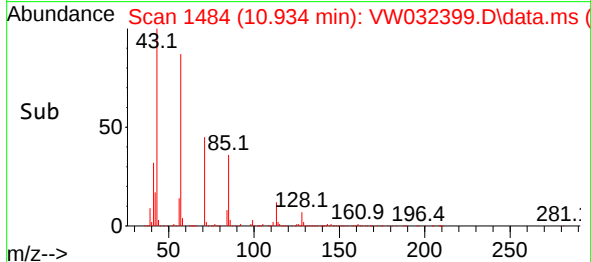

#62
4-Bromofluorobenzene
Concen: 64.839 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 95 Resp: 307677
Ion Ratio Lower Upper
95 100
174 53.9 0.0 145.6
176 54.5 0.0 140.8

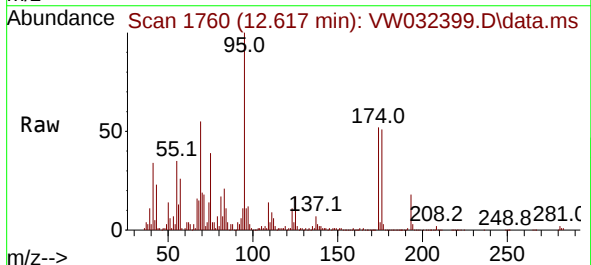



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.635 min Scan# 11

Delta R.T. 0.006 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Instrument :

MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017





Tgt Ion:117 Resp: 508147

Ion Ratio Lower Upper

117 100

82 54.9 42.7 64.1

119 31.2 25.2 37.8

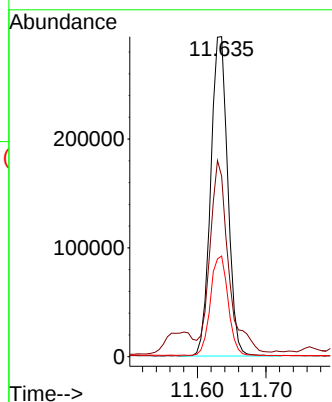

#71

Bromoform

Concen: 4.664 ug/l

RT: 12.282 min Scan# 1705

Delta R.T. -0.067 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58




Tgt Ion:173 Resp: 9310


Ion Ratio Lower Upper

173 100

175 6.0 24.9 74.7#

254 0.0 0.2 0.2#


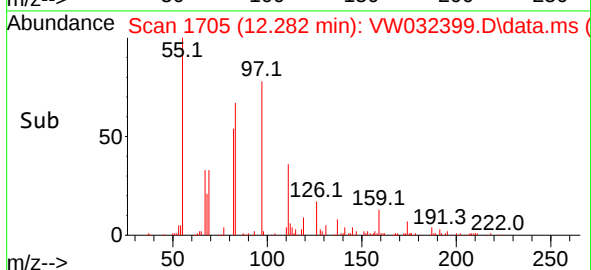






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.556 min Scan# 1914
 Delta R.T. -0.000 min
 Lab File: VW032399.D
 Acq: 20 Oct 2025 18:58




Instrument :
 MSVOA_W
 ClientSampleId :
 PR132-S08-038048-20251017


Tgt Ion:152 Resp: 246462
 Ion Ratio Lower Upper
 152 100
 115 59.4 31.8 95.4
 150 147.4 0.0 343.0

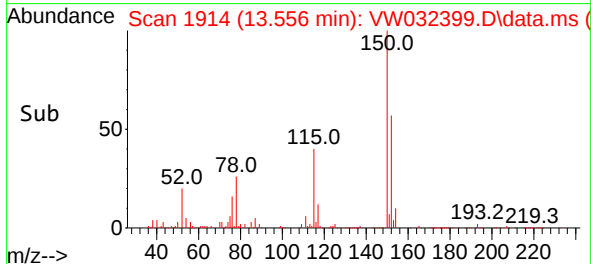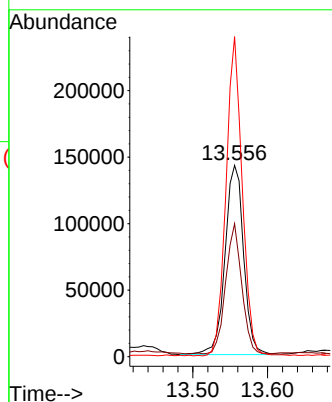

#73
 Isopropylbenzene
 Concen: 1.410 ug/l
 RT: 12.465 min Scan# 1735
 Delta R.T. 0.006 min
 Lab File: VW032399.D
 Acq: 20 Oct 2025 18:58

Tgt Ion:105 Resp: 23774
 Ion Ratio Lower Upper
 105 100
 120 22.6 13.0 38.9

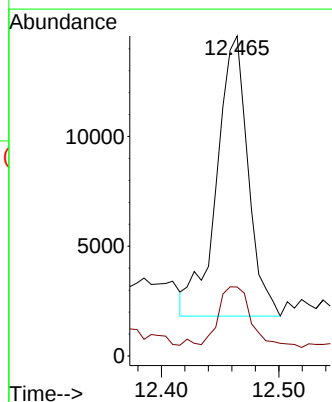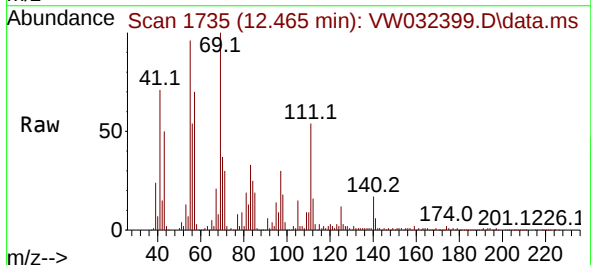



#74

N-amy1 acetate

Concen: 64.631 ug/l

RT: 12.245 min Scan# 1

Delta R.T. -0.024 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Instrument :

MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017

Tgt Ion: 43 Resp: 347663





Ion Ratio Lower Upper

43 100

70 0.0 35.3 52.9#

55 0.0 19.9 29.9#

61 0.0 19.6 29.4#

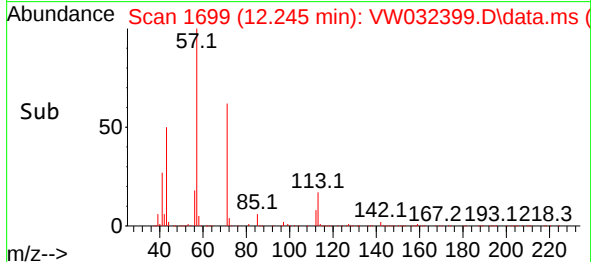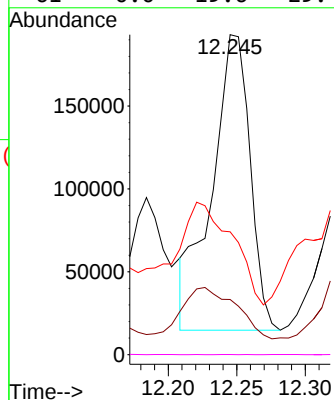

#75

1,1,2,2-Tetrachloroethane

Concen: 8.798 ug/l

RT: 12.684 min Scan# 1771

Delta R.T. -0.031 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58




Tgt Ion: 83 Resp: 36836


Ion Ratio Lower Upper

83 100

131 0.0 5.1 15.4#

85 0.0 32.2 96.6#


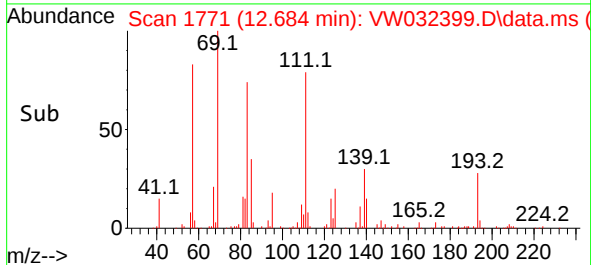
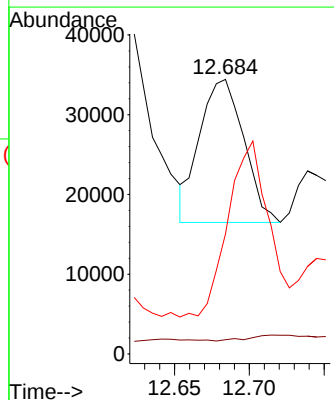





#76
1,2,3-Trichloropropane
Concen: 37.628 ug/l
RT: 12.617 min Scan# 11
Delta R.T. -0.146 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 75 Resp: 122041
Ion Ratio Lower Upper
75 100
77 7.4 141.7 425.1#

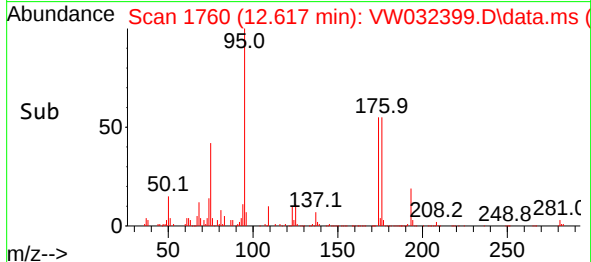

#77
Bromobenzene
Concen: 14.765 ug/l
RT: 12.843 min Scan# 1797
Delta R.T. 0.097 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion:156 Resp: 60015
Ion Ratio Lower Upper
156 100
77 0.0 98.6 295.7#
158 1.0 48.4 145.0#




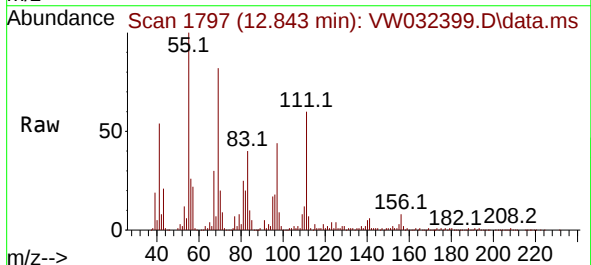




#81
trans-1,4-Dichloro-2-butene
Concen: 95.323 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.104 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58




Instrument :
MSVOA_W
ClientSampleId :
PR132-S08-038048-20251017


Tgt Ion: 75 Resp: 122041
Ion Ratio Lower Upper
75 100
53 11.0 91.0 136.6#
89 0.0 39.4 59.2#

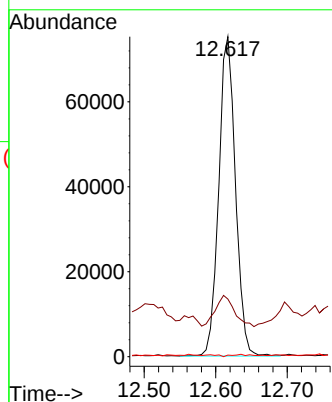

#84
1,2,4-Trimethylbenzene
Concen: 1.185 ug/l
RT: 13.251 min Scan# 1864
Delta R.T. 0.006 min
Lab File: VW032399.D
Acq: 20 Oct 2025 18:58

Tgt Ion: 105 Resp: 17571
Ion Ratio Lower Upper
105 100
120 30.5 22.1 66.3

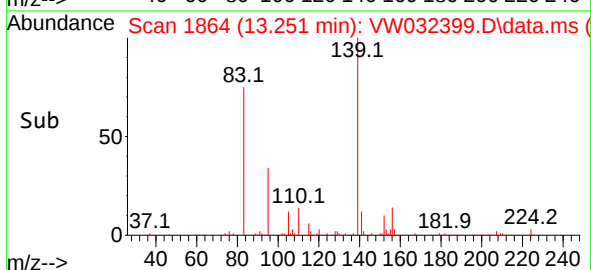



#92

1,2-Dibromo-3-Chloropropane

Concen: 1.121 ug/l

RT: 14.263 min Scan# 2066

Delta R.T. -0.220 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58

Instrument :

MSVOA_W

ClientSampleId :

PR132-S08-038048-20251017





Tgt Ion: 75 Resp: 822

Ion Ratio Lower Upper

75 100

155 74.3 40.8 122.5

157 101.8 51.8 155.4

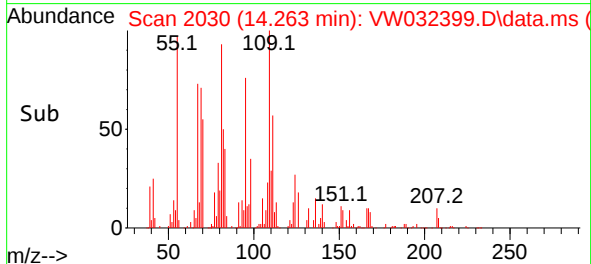

#95

Naphthalene

Concen: 1.018 ug/l

RT: 15.360 min Scan# 2210

Delta R.T. -0.000 min

Lab File: VW032399.D

Acq: 20 Oct 2025 18:58




Tgt Ion: 128 Resp: 10910


Ion Ratio Lower Upper

128 100

127 0.0 10.6 16.0#


129 4.5 8.4 12.6#





#96
 1,2,3-Trichlorobenzene
 Concen: 1.960 ug/l
 RT: 15.513 min Scan# 21
 Delta R.T. -0.031 min
 Lab File: VW032399.D
 Acq: 20 Oct 2025 18:58

Instrument :
 MSVOA_W
 ClientSampleId :
 PR132-S08-038048-20251017

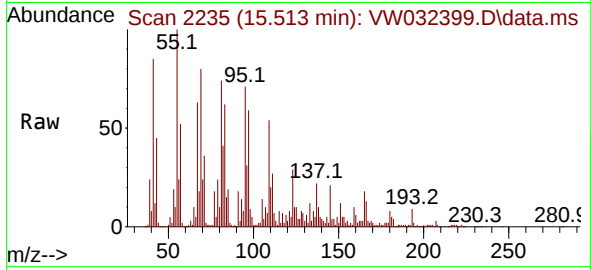

Tgt Ion:180 Resp: 8242
 Ion Ratio Lower Upper
 180 100
 182 22.2 47.7 143.1#
 145 253.0 17.2 51.6#

