

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030678.D
 Acq On : 21 Oct 2024 11:30
 Operator : SY/MD
 Sample : P44413-23
 Misc : 5.31g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 22 01:34:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	284012	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	270102	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	117613	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	72196	16.172	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.680%
7) Chloroethane-d5	2.899	69	64856	19.192	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.760%
11) 1,1-Dichloroethene-d2	4.009	65	30973	16.681	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.720%
21) 2-Butanone-d5	7.069	46	36423	45.336	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.680%
24) Chloroform-d	7.648	84	163620	20.145	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.560%
26) 1,2-Dichloroethane-d4	8.301	65	88331	20.914	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.640%
32) Benzene-d6	8.270	84	290693	18.543	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.160%
36) 1,2-Dichloropropane-d6	9.270	67	93769	20.379	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.520%
41) Toluene-d8	10.319	98	262653	18.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.400%
43) trans-1,3-Dichloroprop...	10.575	79	35445	18.397	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.600%
47) 2-Hexanone-d5	10.922	63	25476	42.987	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75107	22.227	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.920%
66) 1,2-Dichlorobenzene-d4	13.848	152	90045	22.627	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3390	0.512	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030678.D
Acq On : 21 Oct 2024 11:30
Operator : SY/MD
Sample : P44413-23
Misc : 5.31g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 22 01:34:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 22 01:33:40 2024
Response via : Initial Calibration

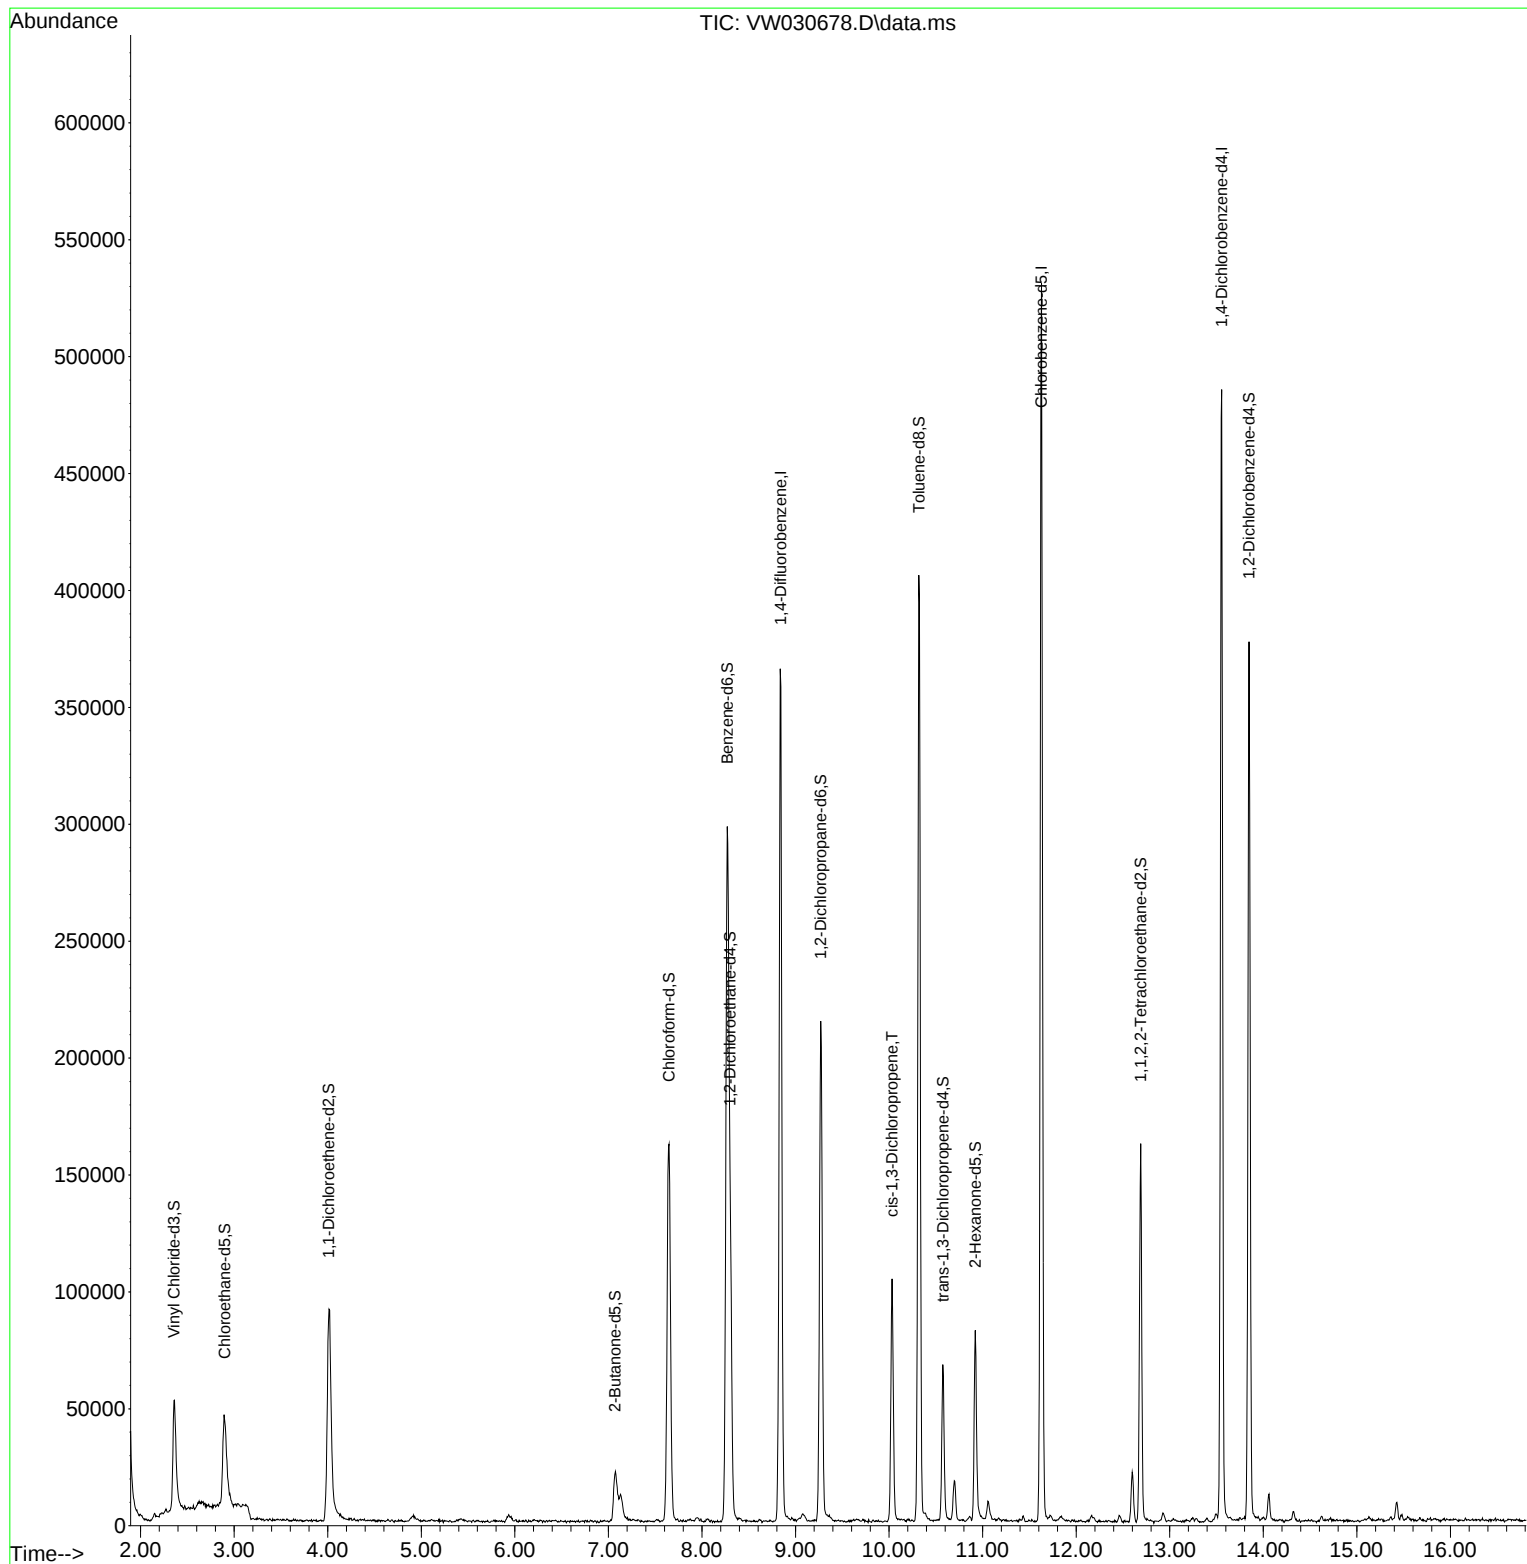

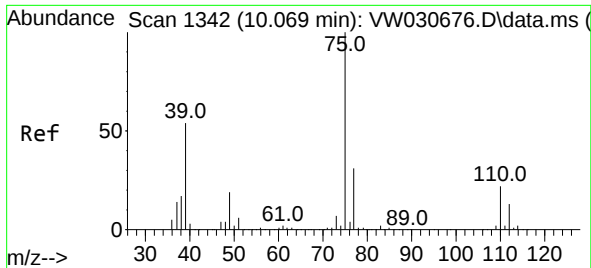

#39
 cis-1,3-Dichloropropene
 Concen: 0.512 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030678.D
 Acq: 21 Oct 2024 11:30

Instrument :
 MSVOA_W
 ClientSampleId :

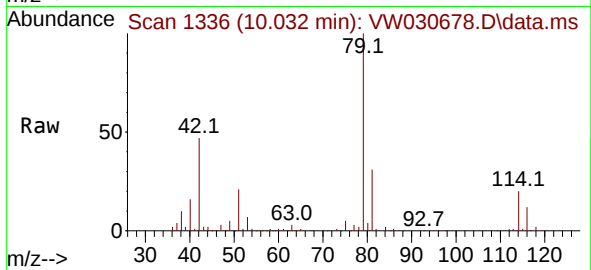

Tgt Ion: 75 Resp: 3390
 Ion Ratio Lower Upper
 75 100
 77 52.4 21.1 39.1#

