

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030679.D
 Acq On : 21 Oct 2024 11:54
 Operator : SY/MD
 Sample : P4429-13
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 22 01:34:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	292557	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	278197	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	125091	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64928	14.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.480%
7) Chloroethane-d5	2.905	69	59979	17.231	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.920%
11) 1,1-Dichloroethene-d2	4.021	65	27348	14.298	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.200%
21) 2-Butanone-d5	7.081	46	33259	40.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.380%
24) Chloroform-d	7.648	84	152877	18.272	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.080%
26) 1,2-Dichloroethane-d4	8.307	65	81988	18.845	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.400%
32) Benzene-d6	8.276	84	269357	16.682	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	66.720%
36) 1,2-Dichloropropane-d6	9.270	67	87590	18.482	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.920%
41) Toluene-d8	10.325	98	241433	16.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.520%
43) trans-1,3-Dichloroprop...	10.575	79	32205	16.229	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.920%
47) 2-Hexanone-d5	10.922	63	24211	39.664	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	70408	20.230	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.920%
66) 1,2-Dichlorobenzene-d4	13.848	152	83699	19.775	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.120%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3136	0.460	ug/L	Qvalue # 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030679.D
Acq On : 21 Oct 2024 11:54
Operator : SY/MD
Sample : P4429-13
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 22 01:34:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 22 01:33:40 2024
Response via : Initial Calibration

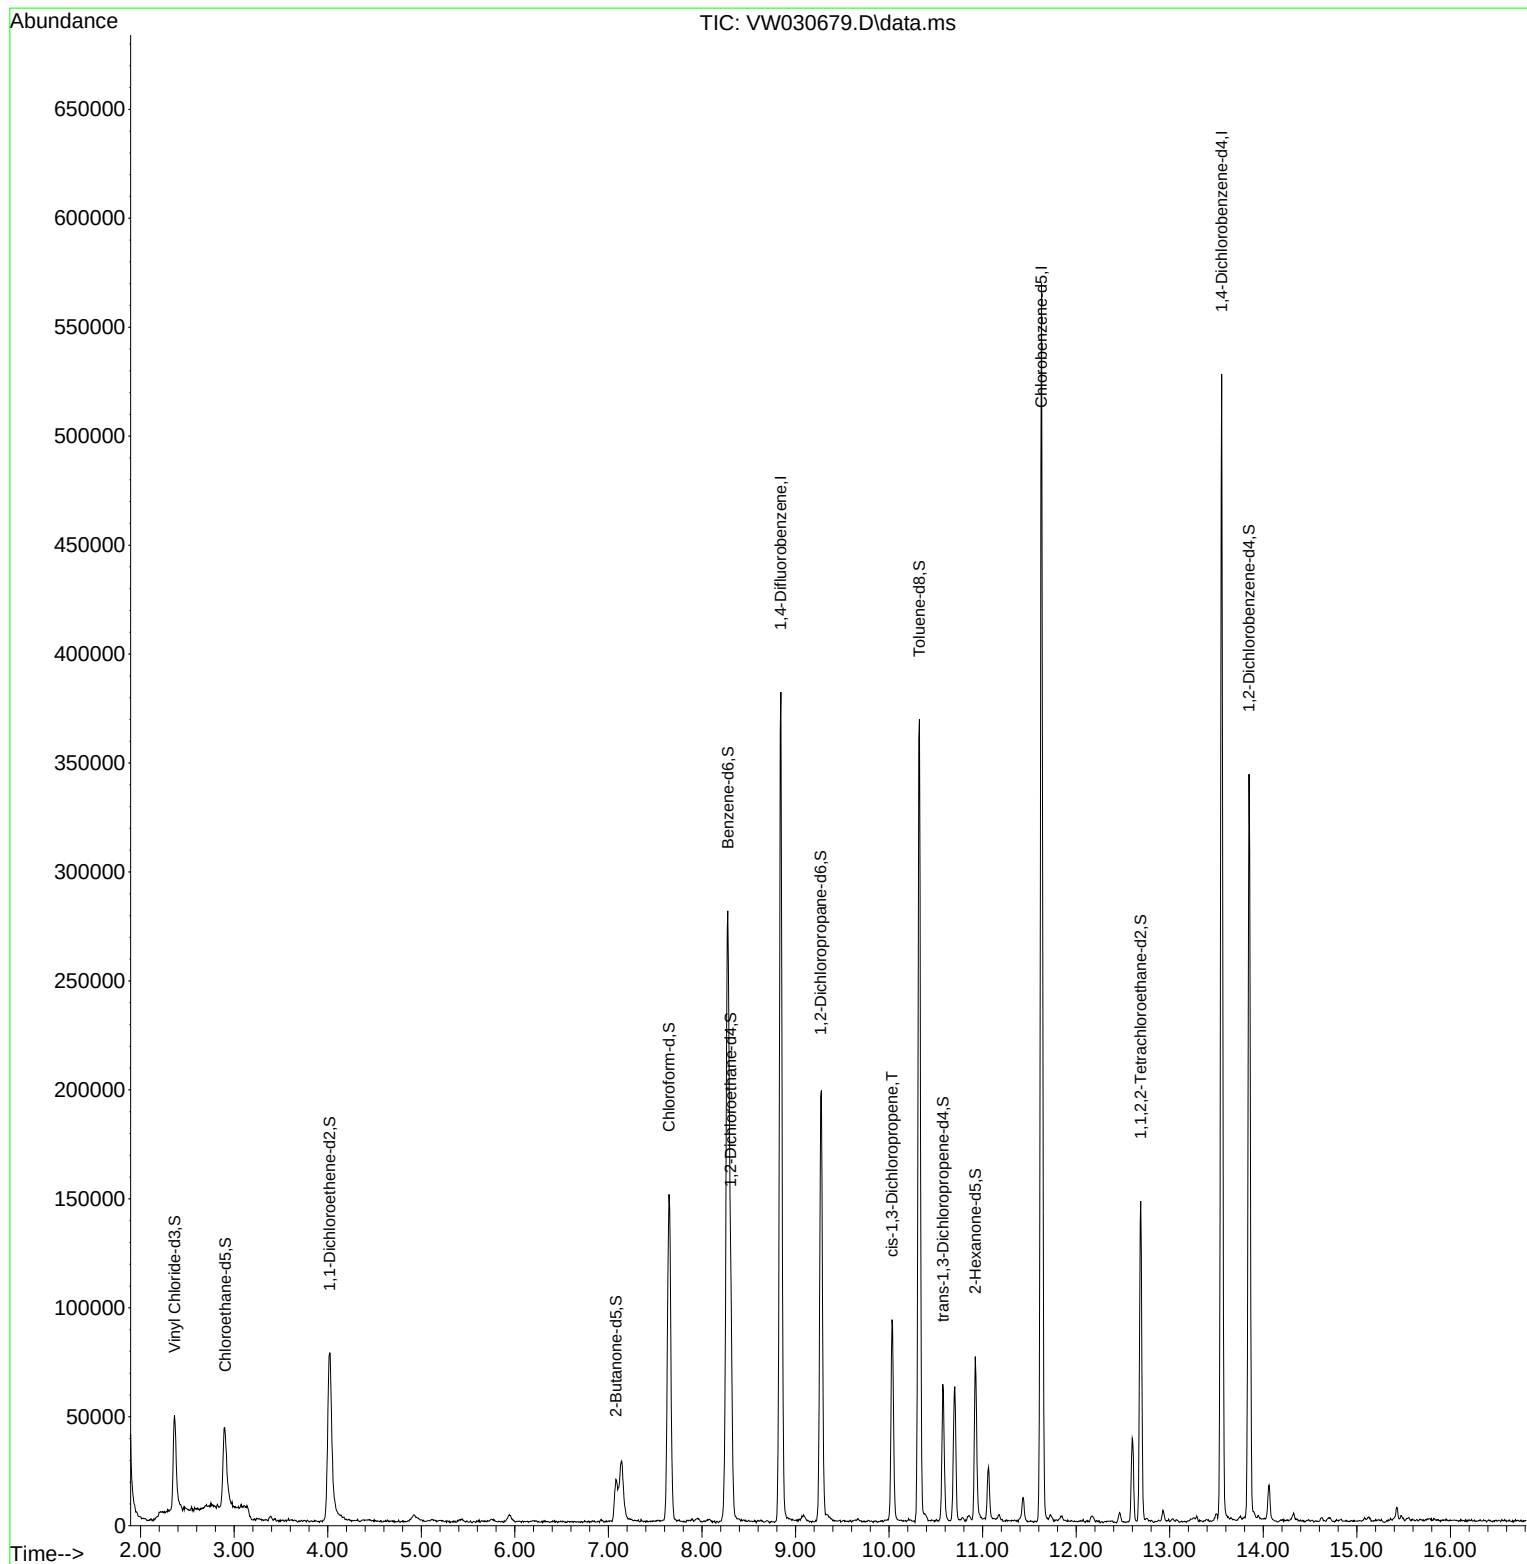

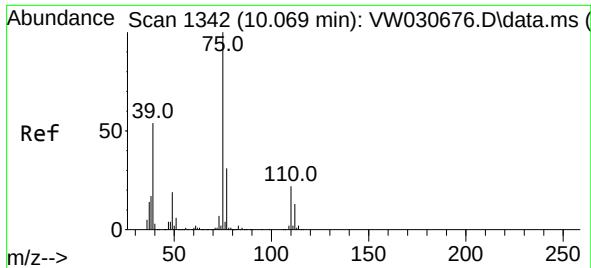

#39
 cis-1,3-Dichloropropene
 Concen: 0.460 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030679.D
 Acq: 21 Oct 2024 11:54

Instrument :
 MSVOA_W
 ClientSampleId :

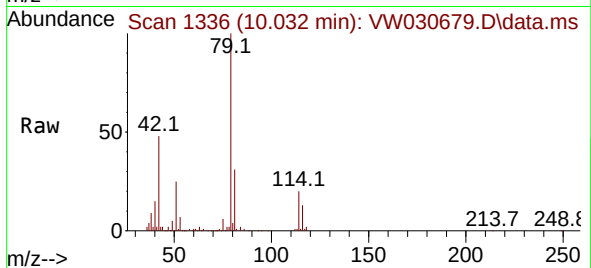

Tgt Ion: 75 Resp: 3136
 Ion Ratio Lower Upper
 75 100
 77 45.1 21.1 39.1#

